

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

FIG. 1

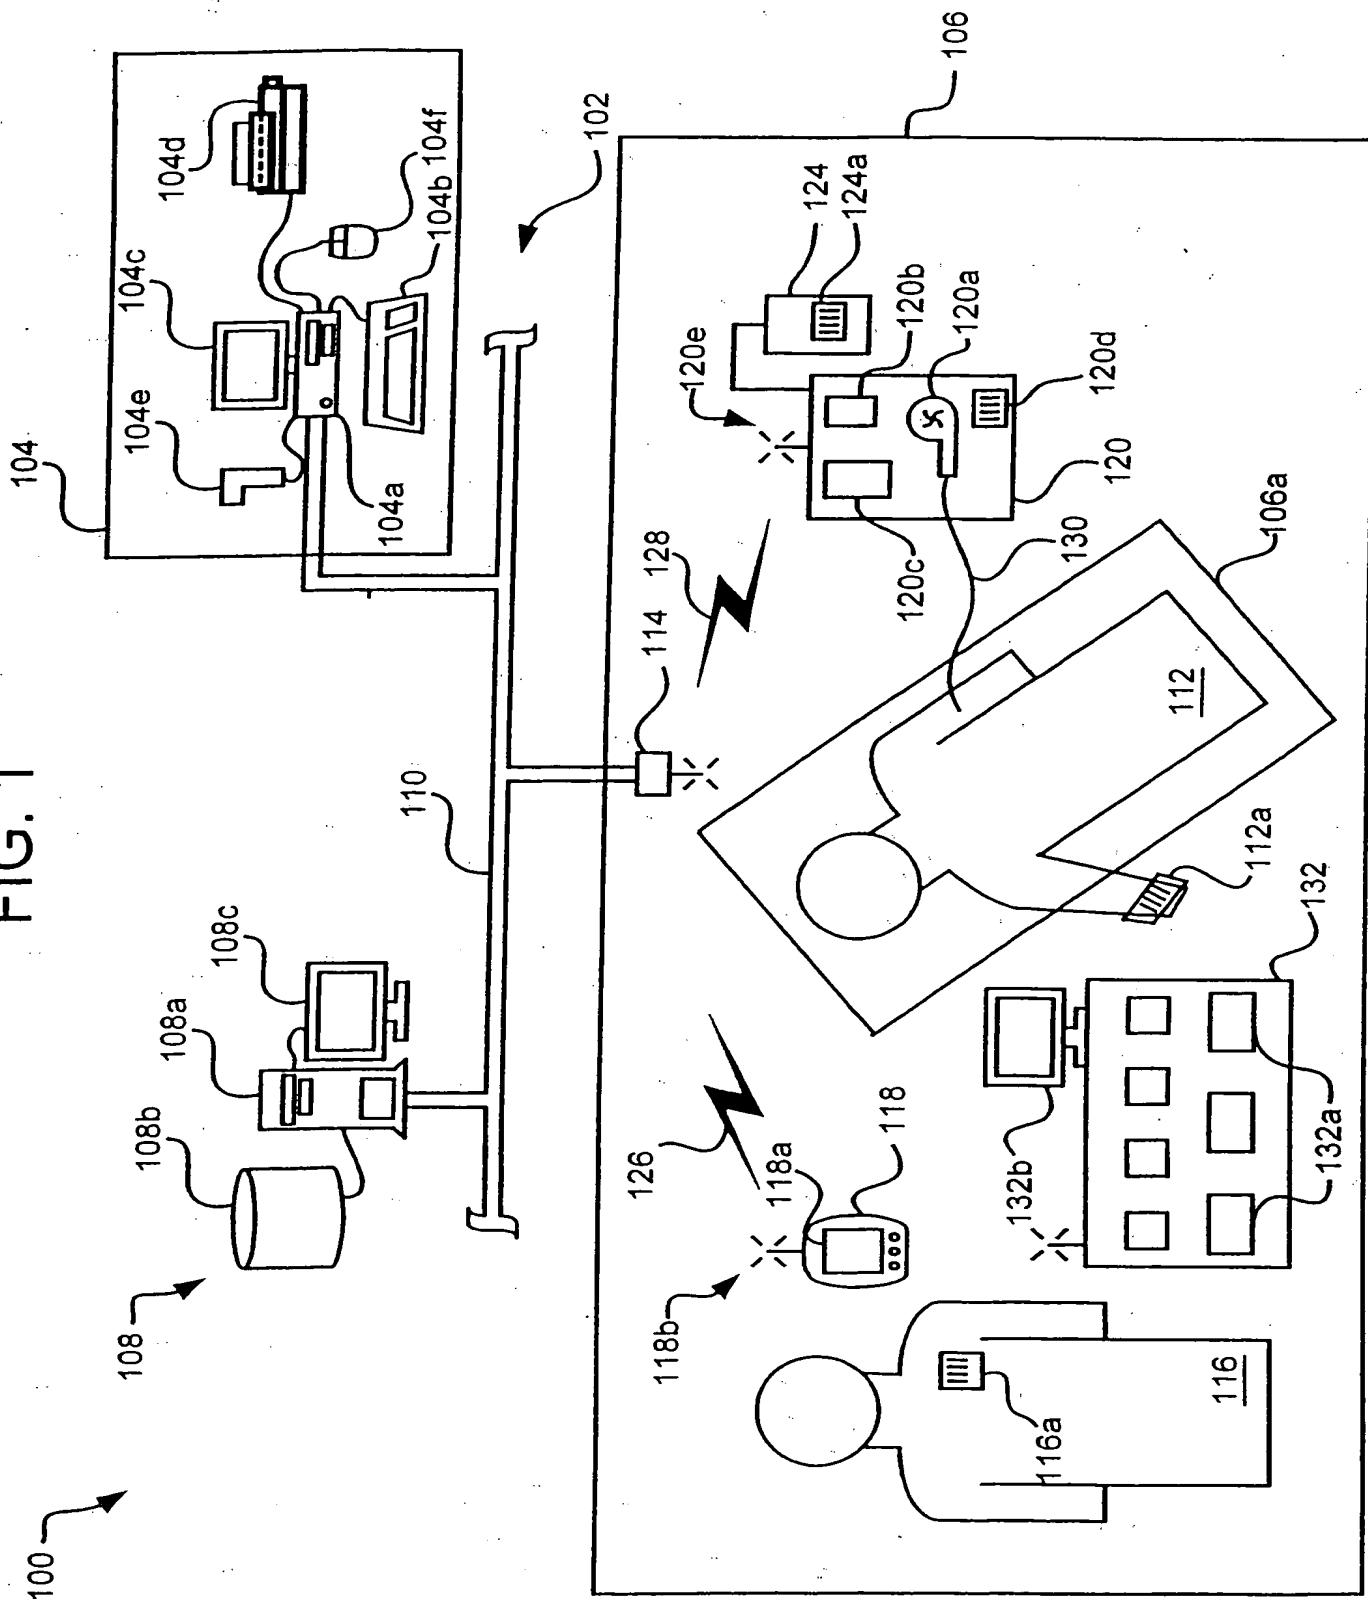


FIG. 2

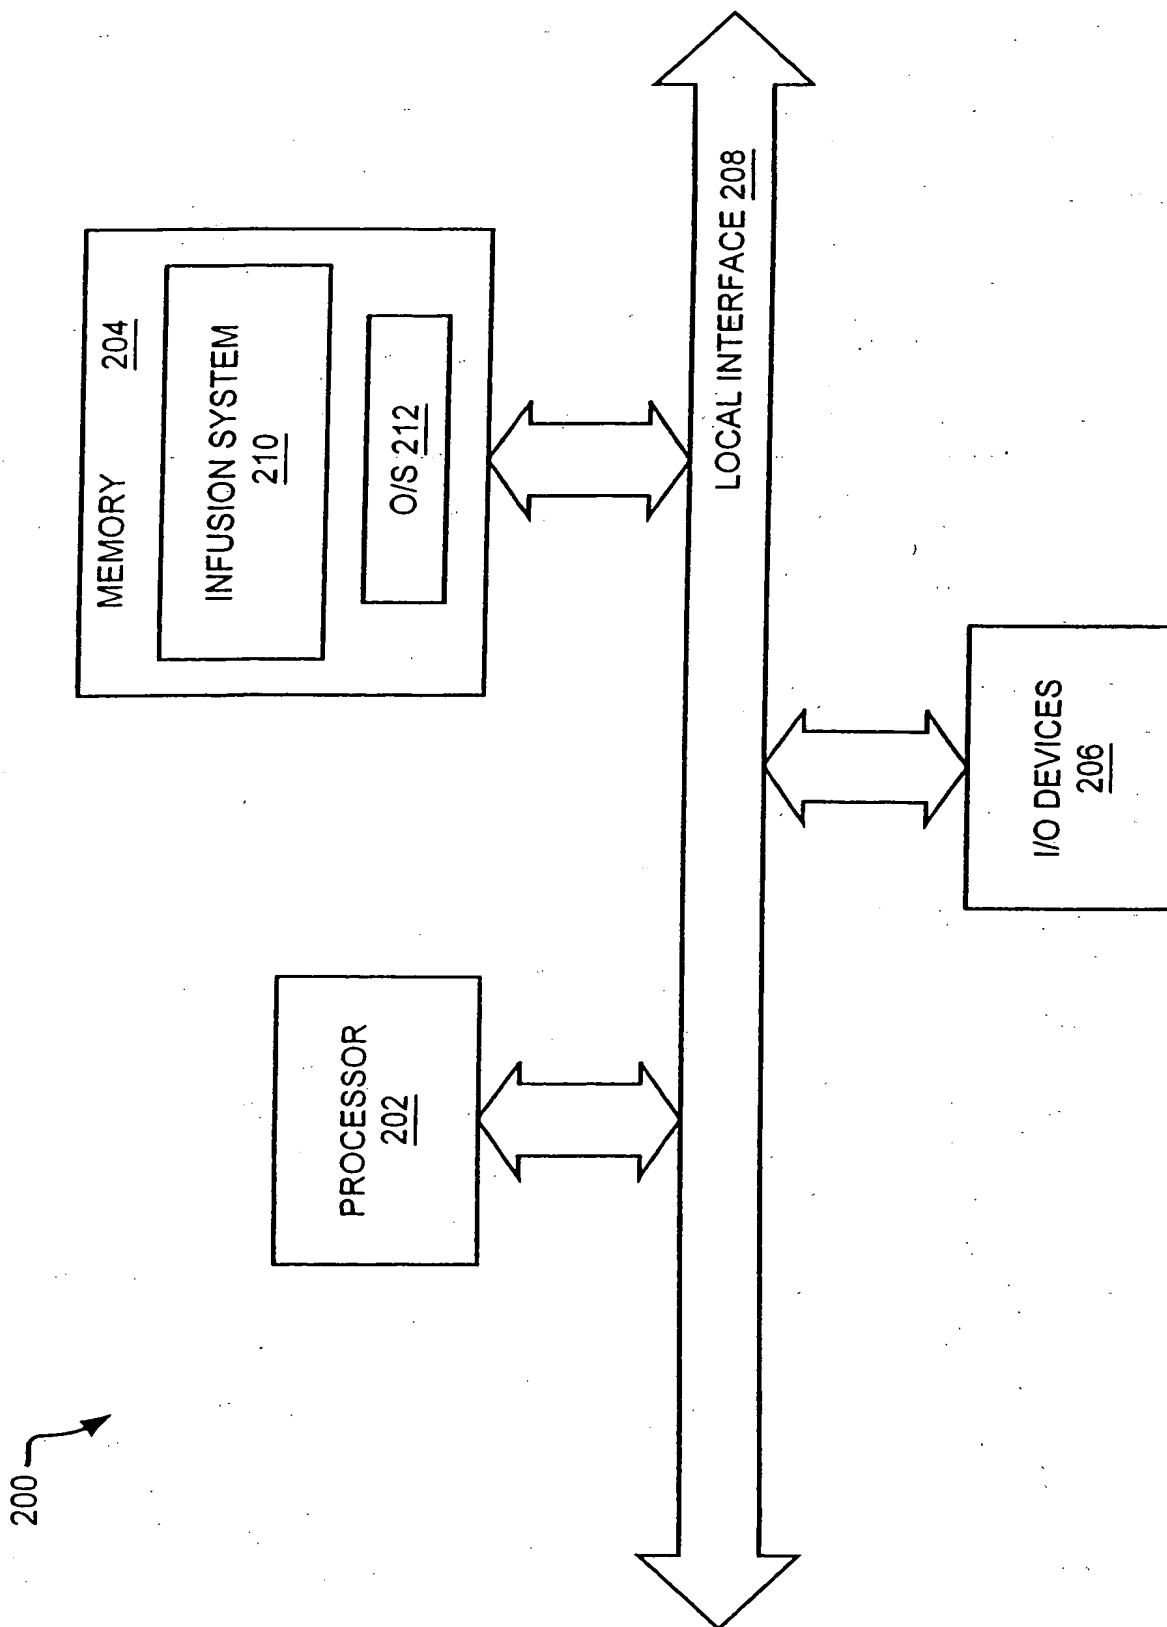
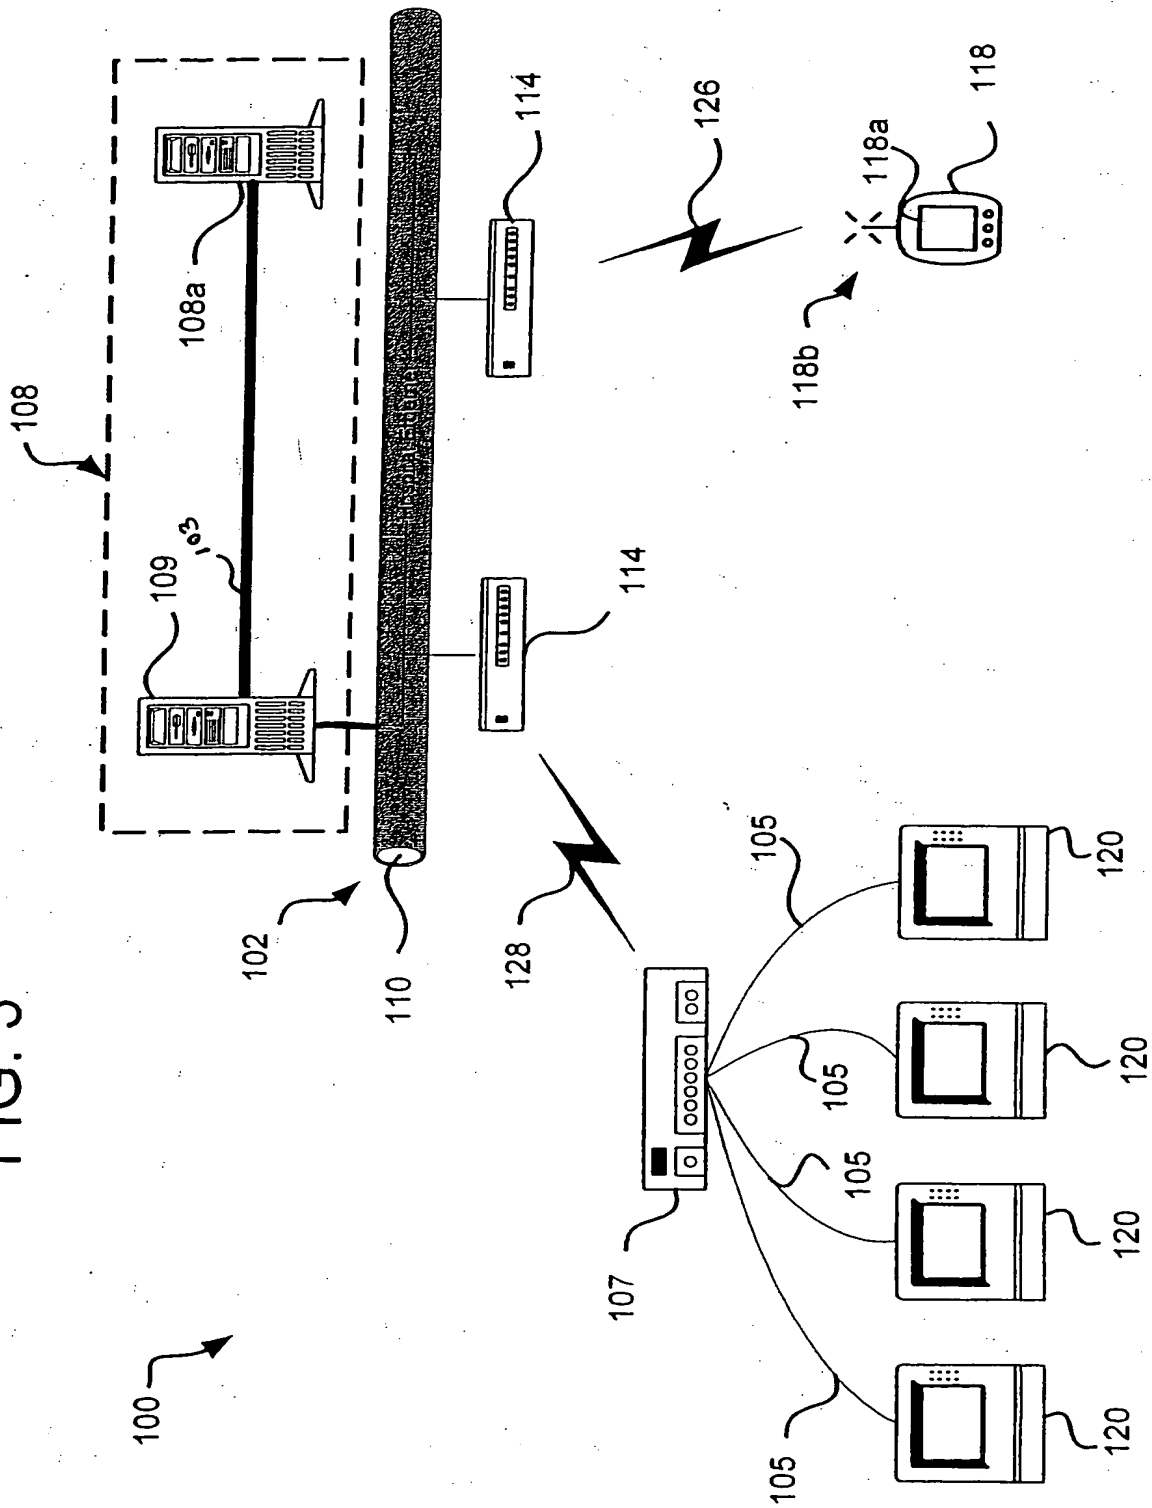


FIG. 3



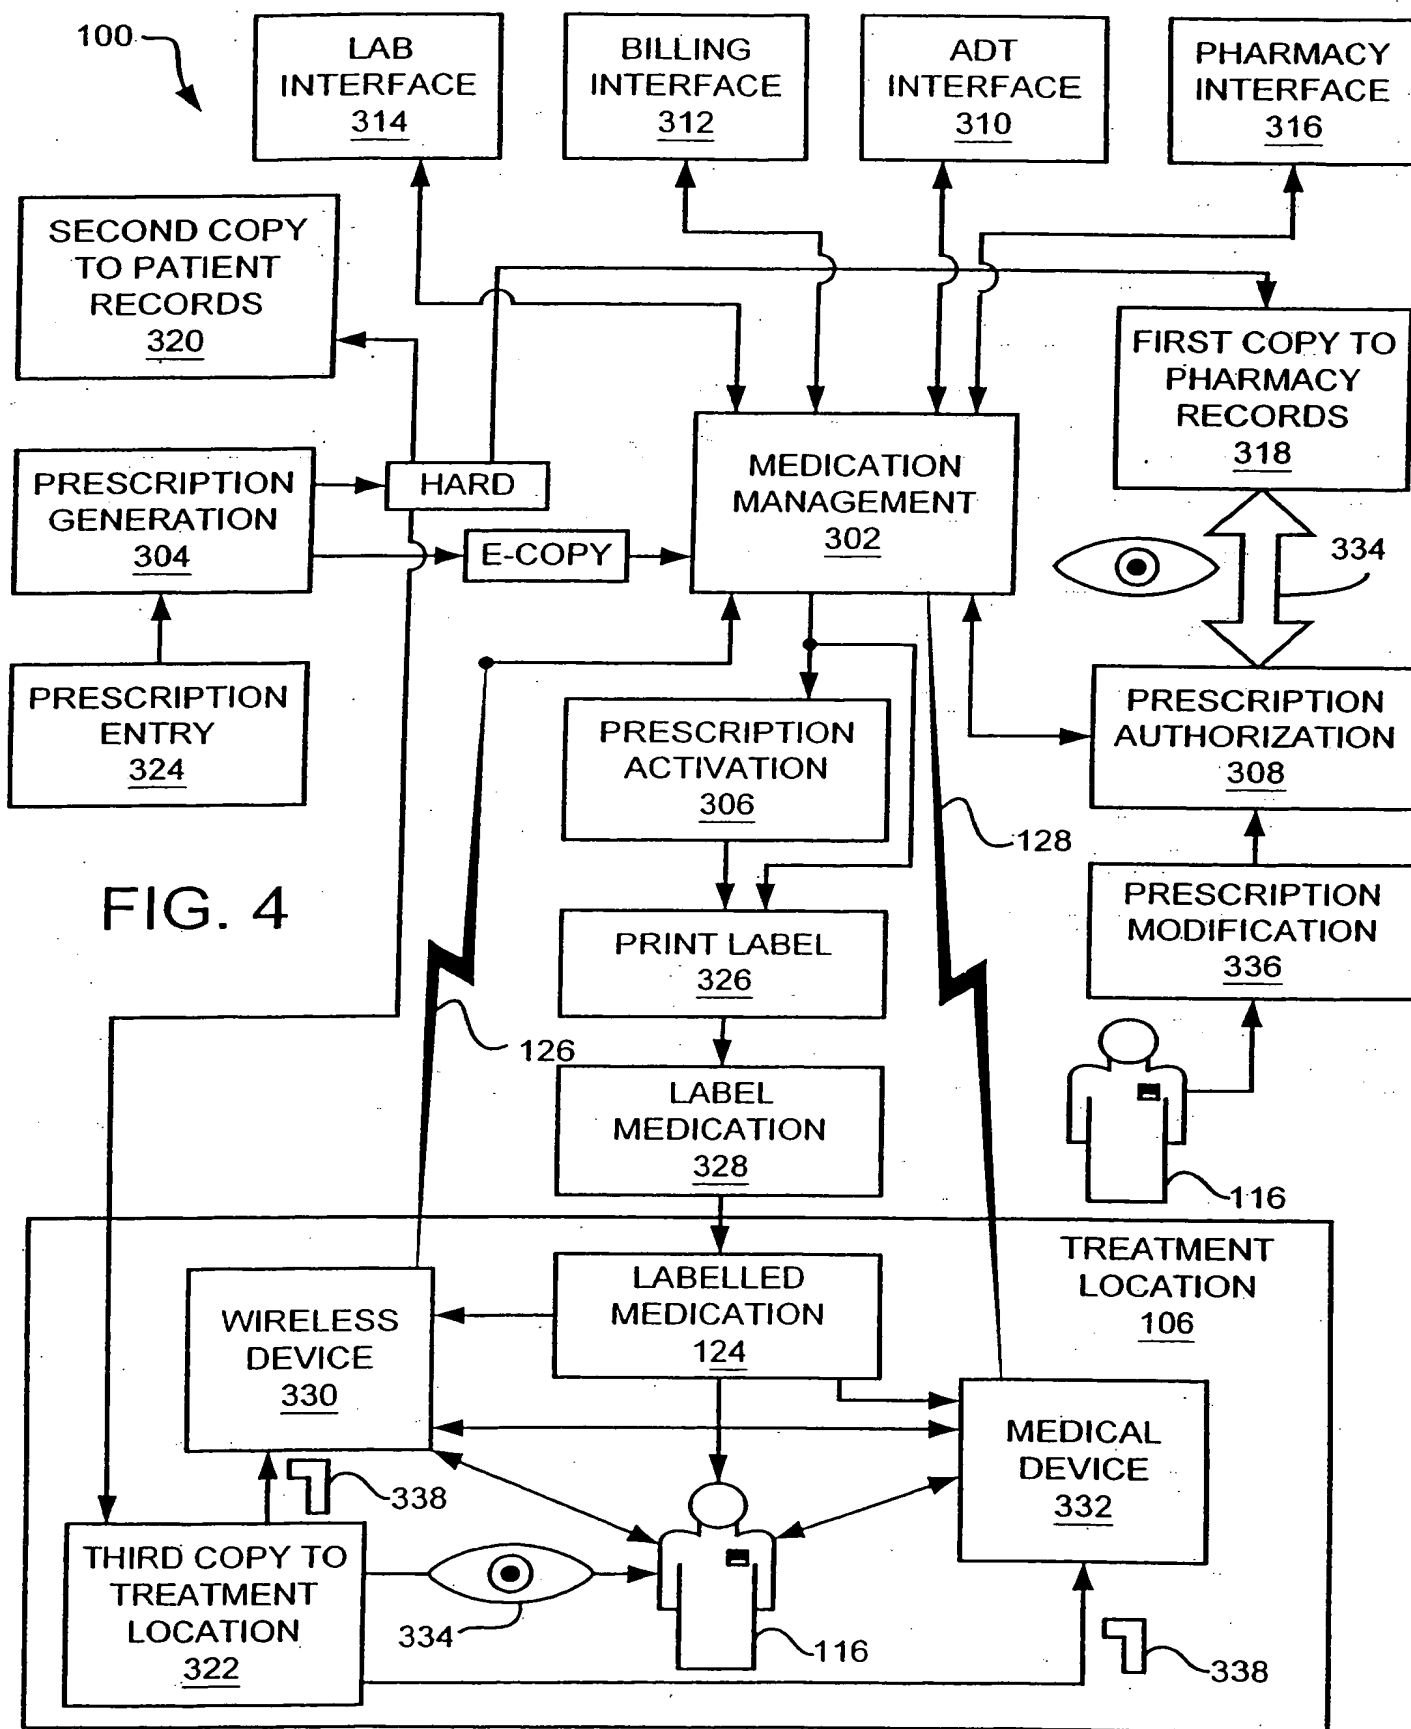


FIG. 5

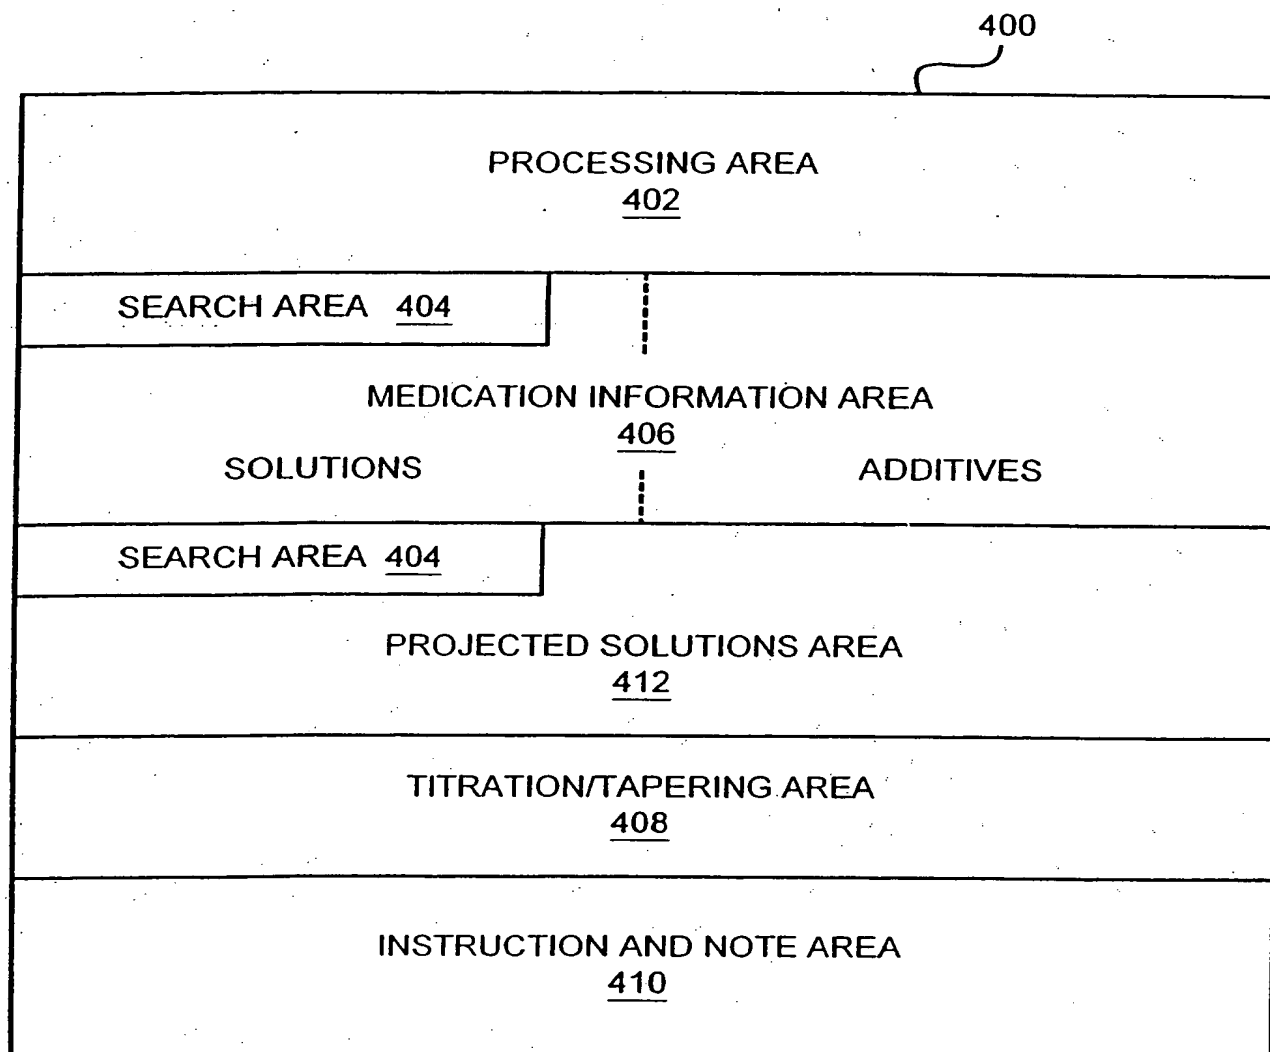
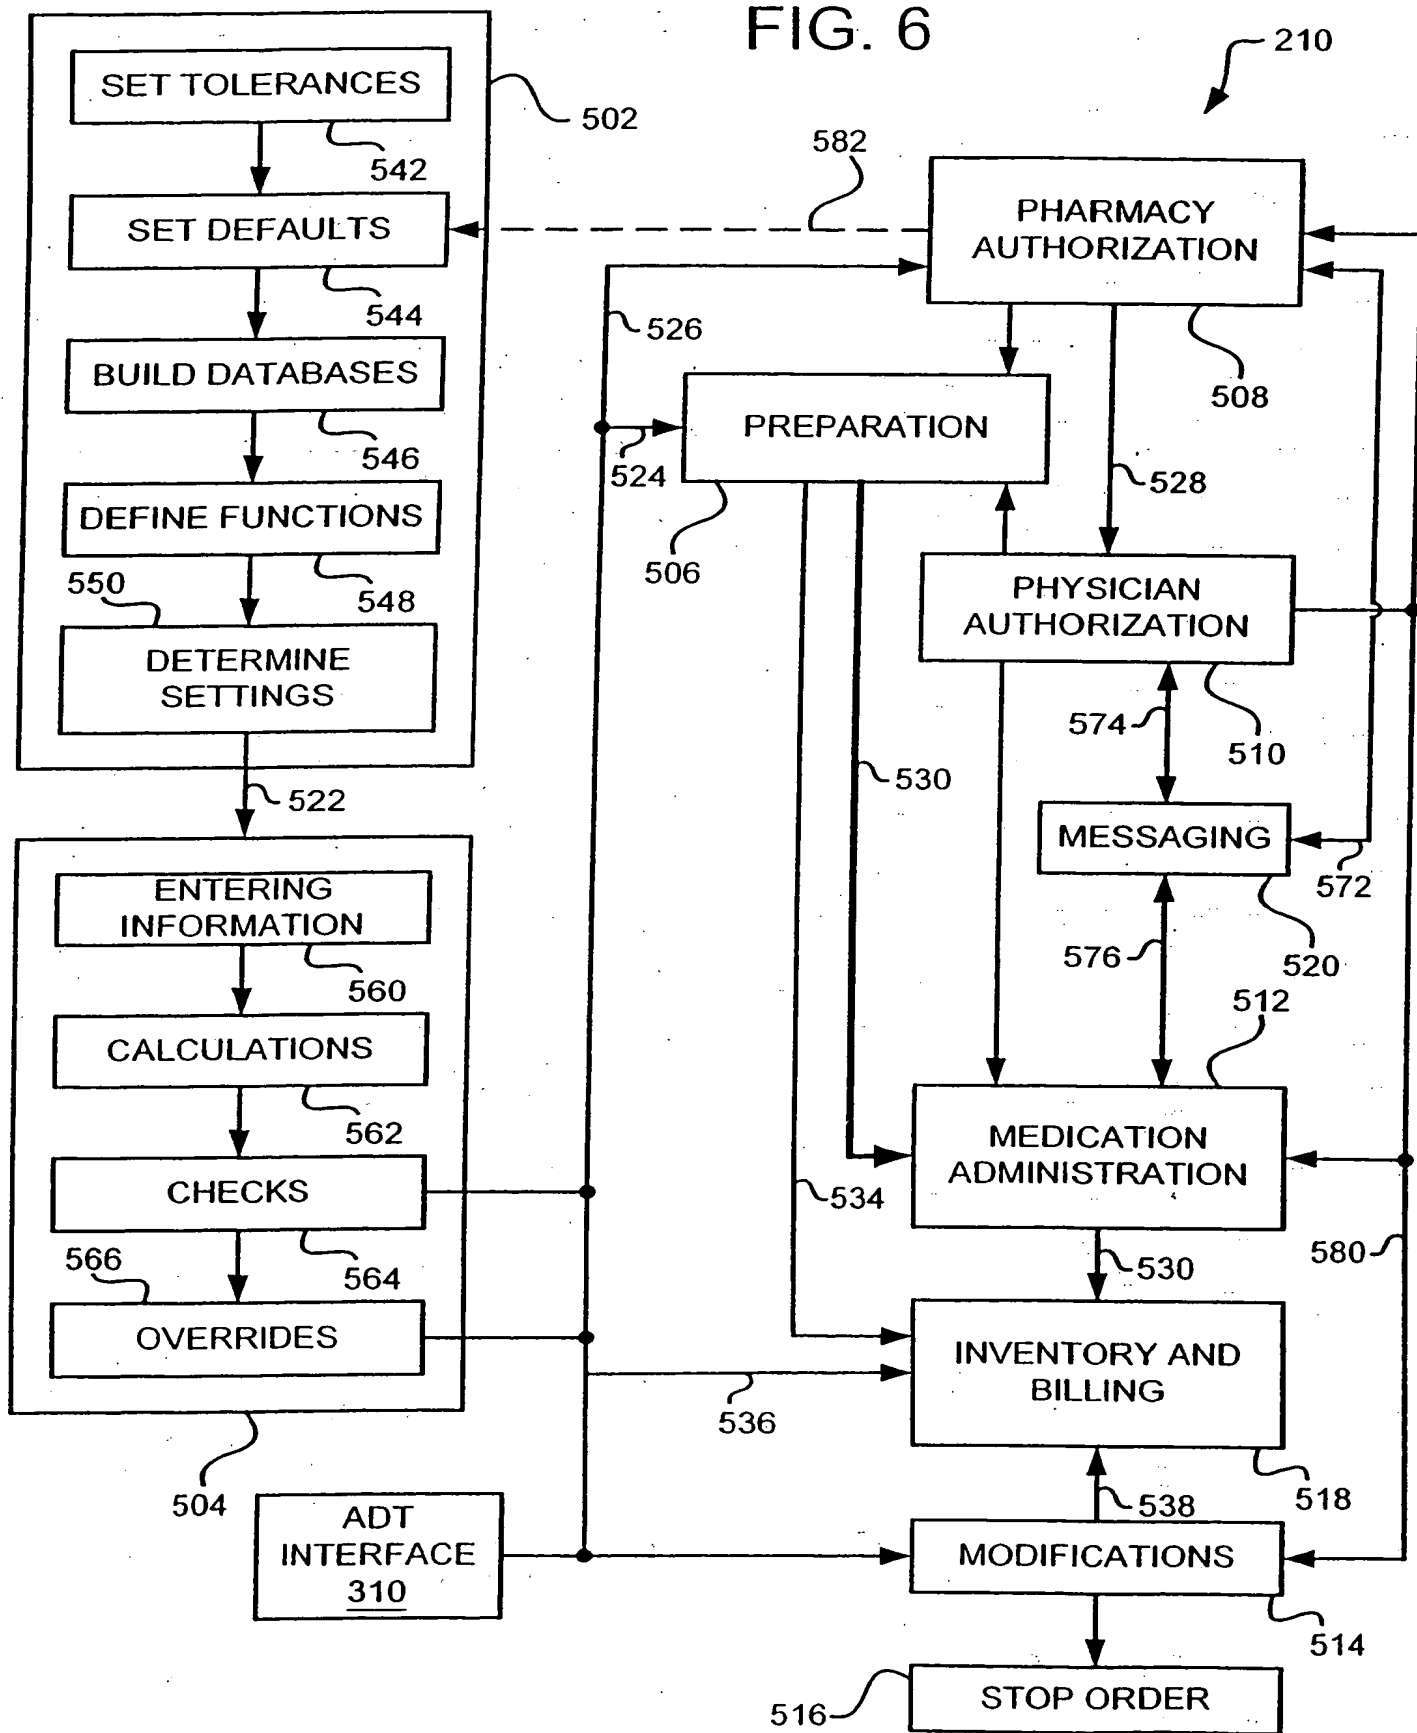


FIG. 6



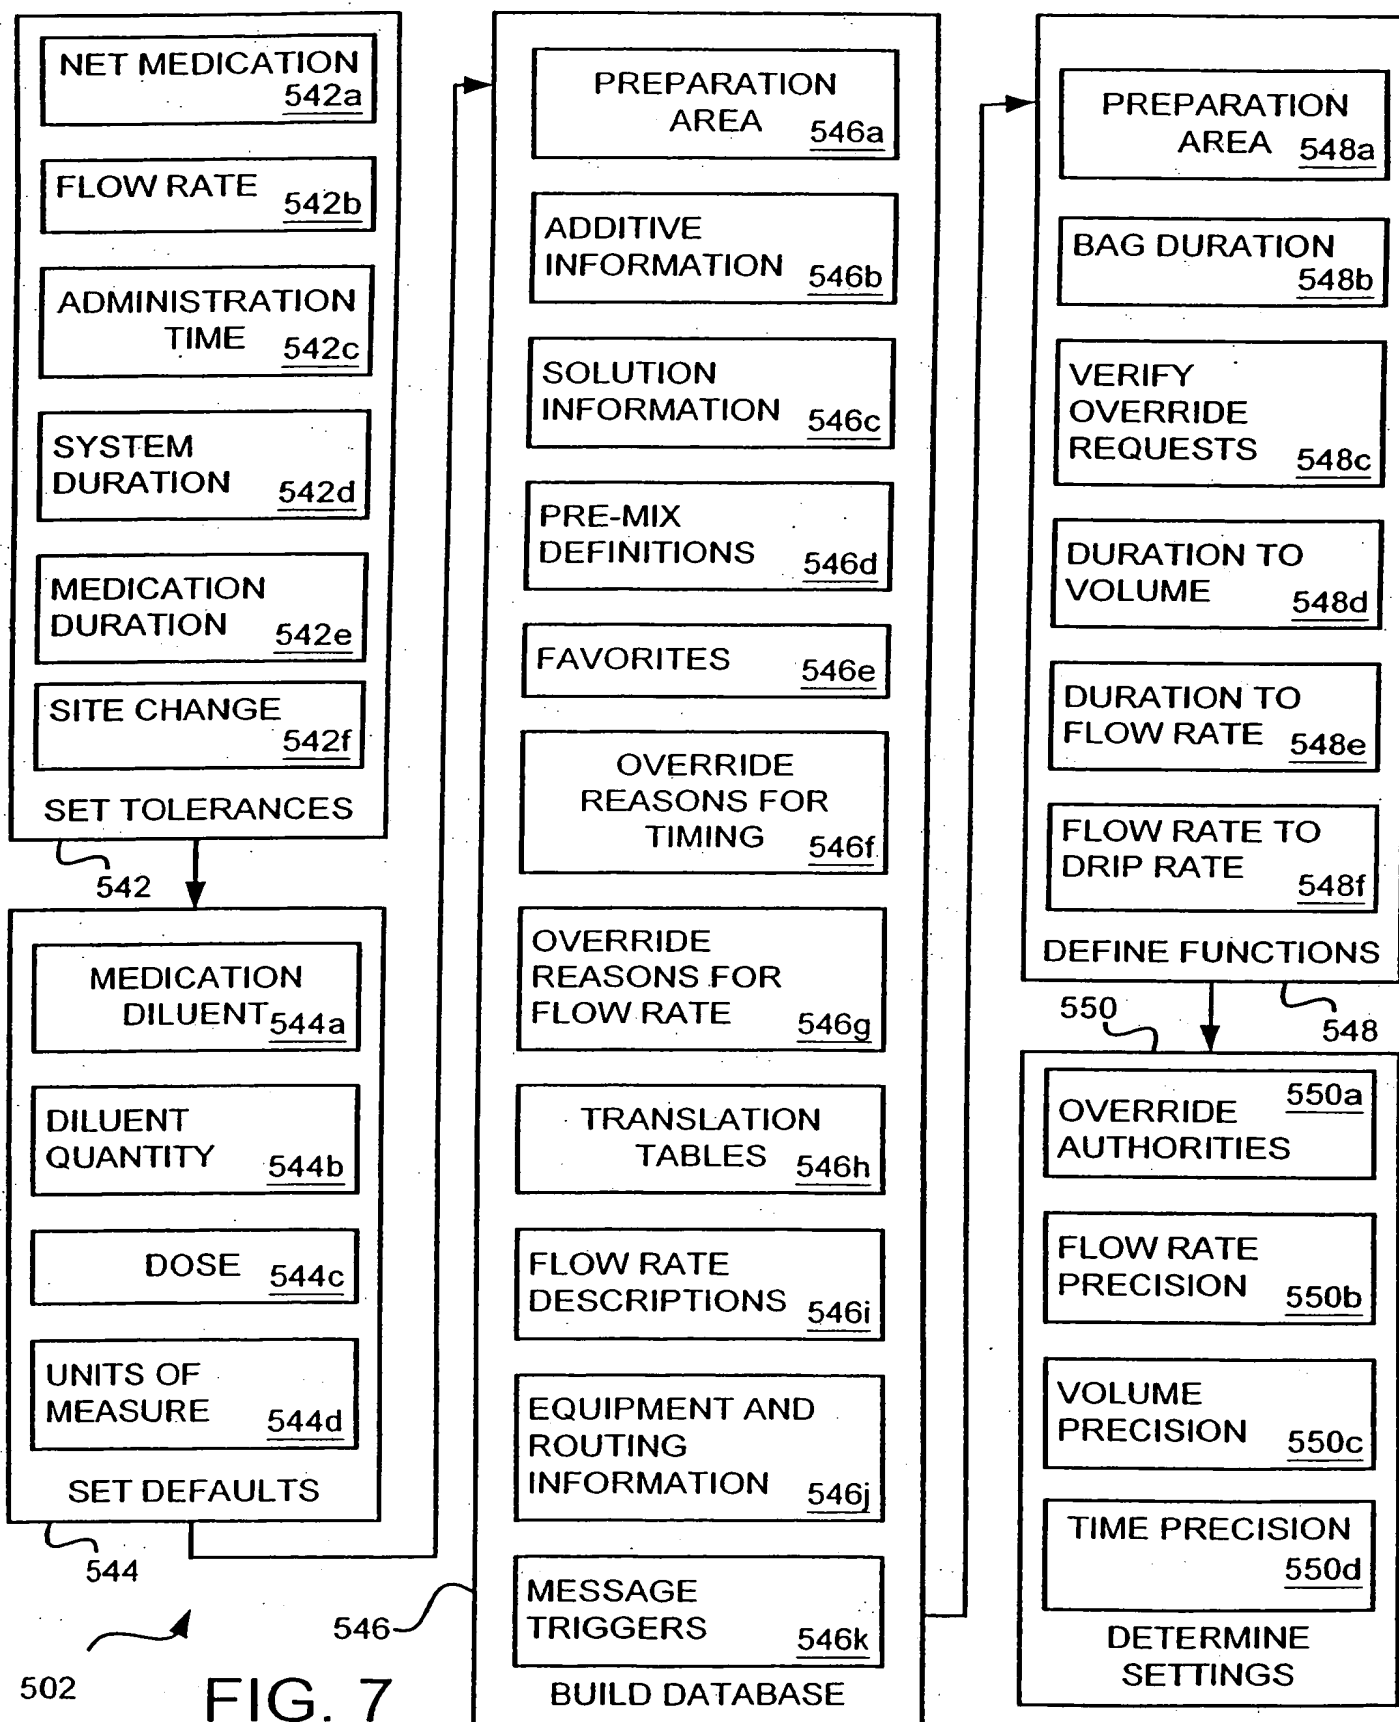


FIG. 7

FIG. 8

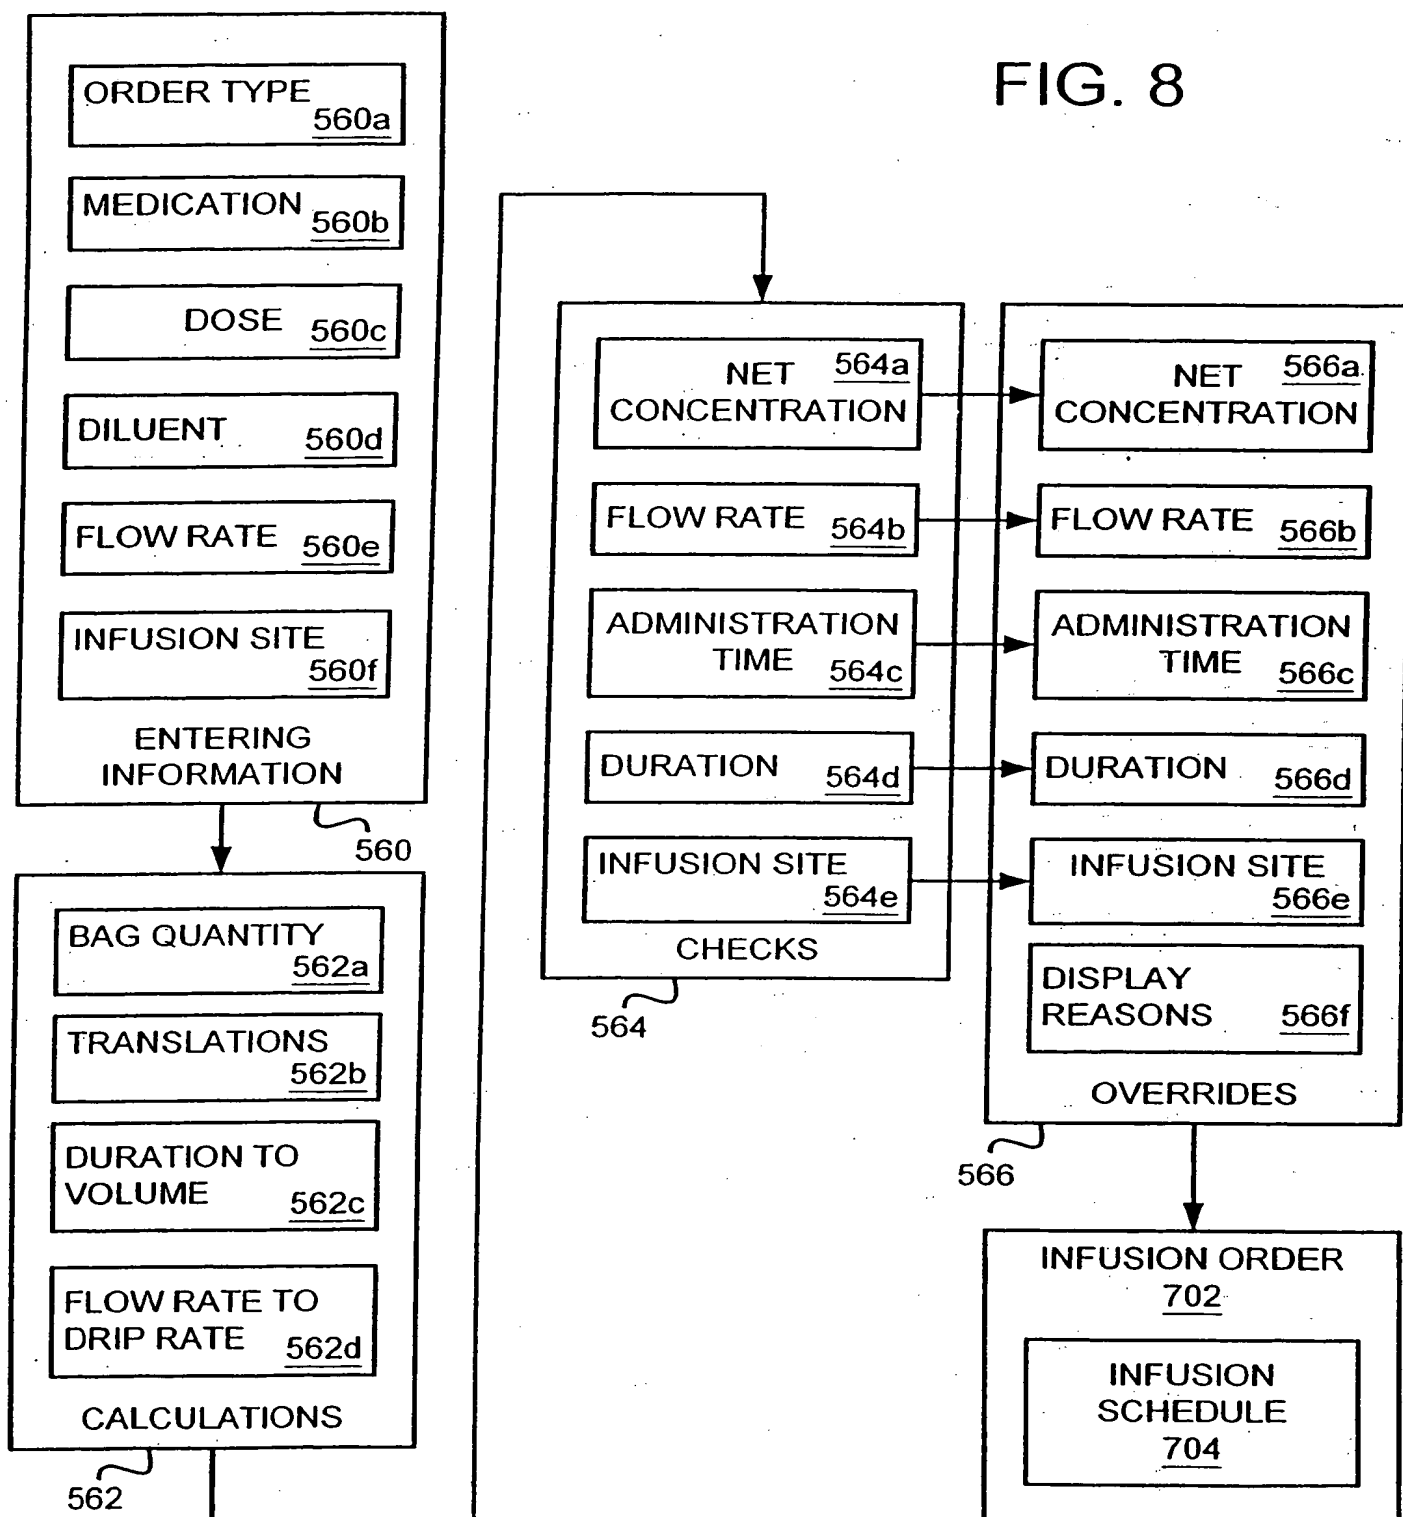


FIG. 9

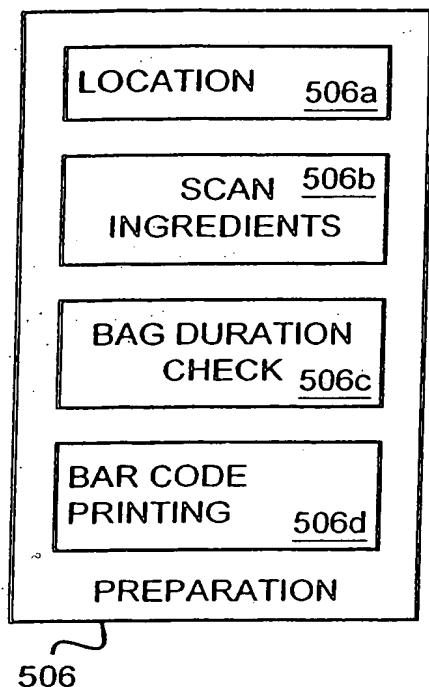


FIG. 10

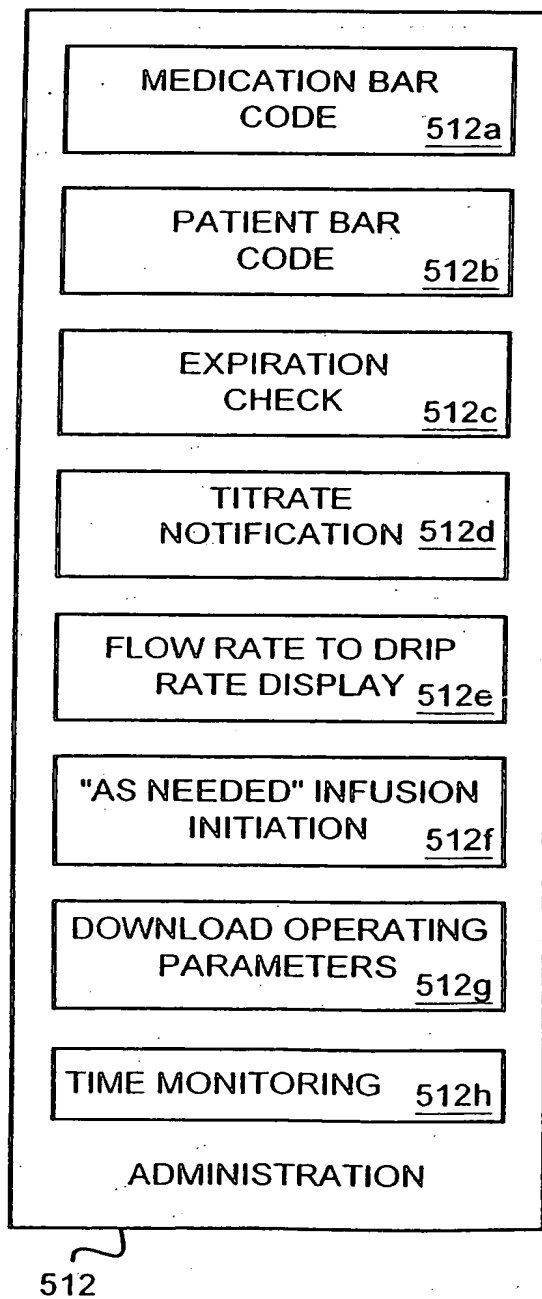
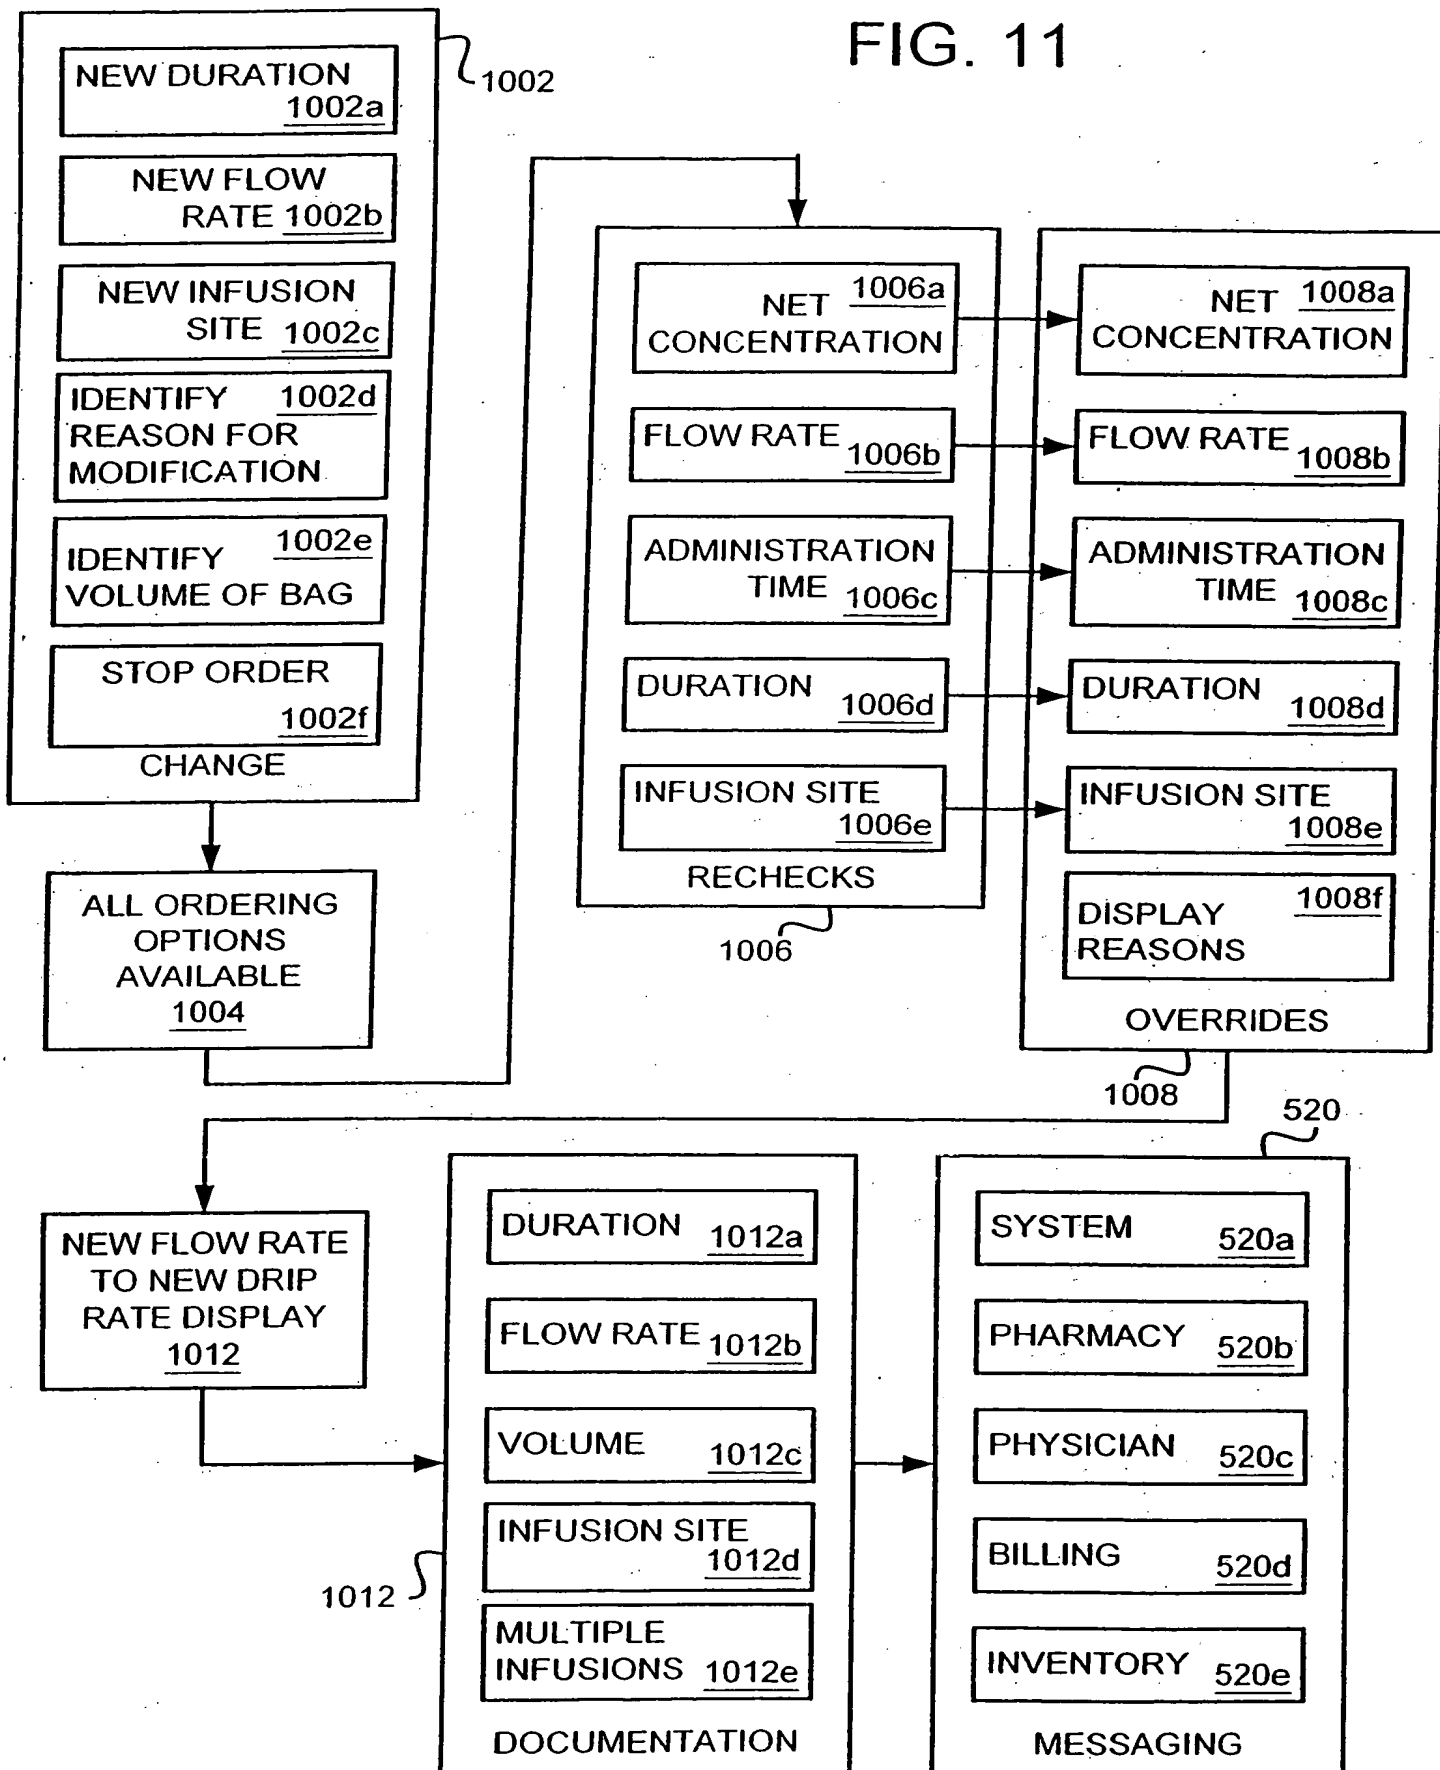


FIG. 11



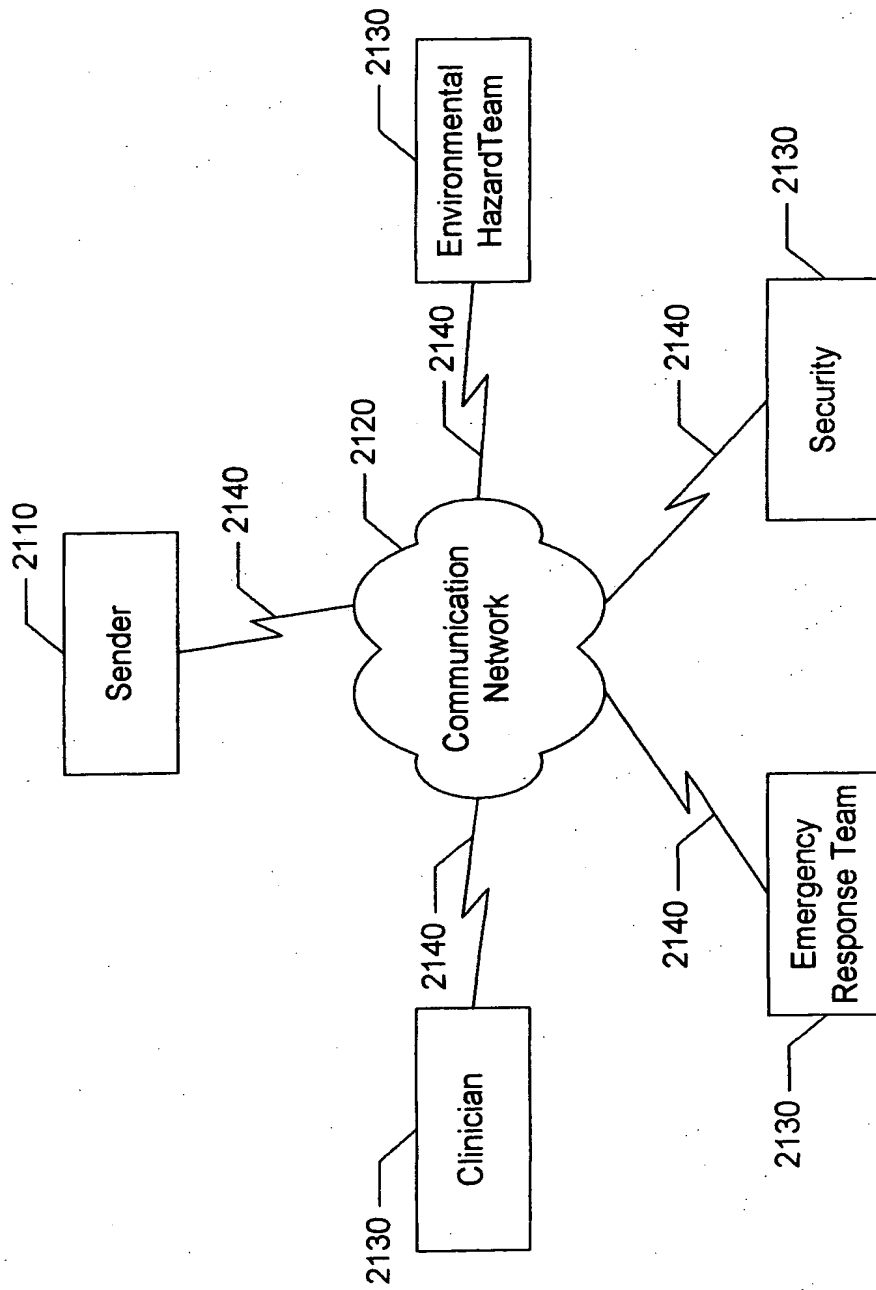


FIG. 12

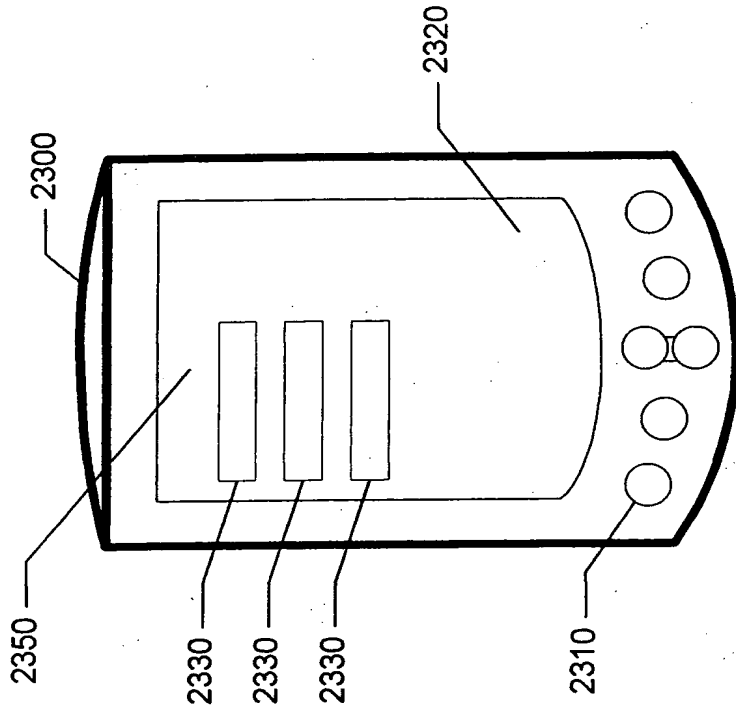


FIG. 13

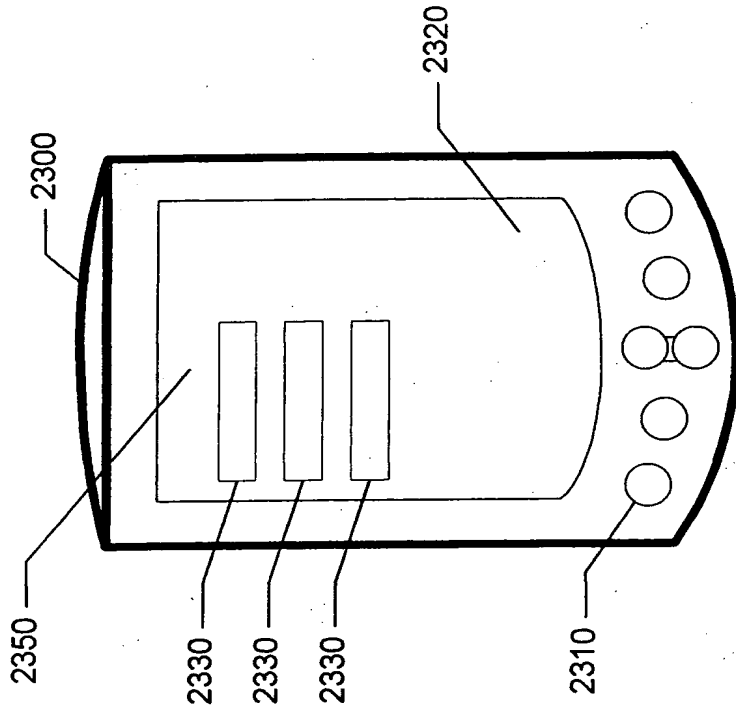


FIG. 14

FIGURE 15

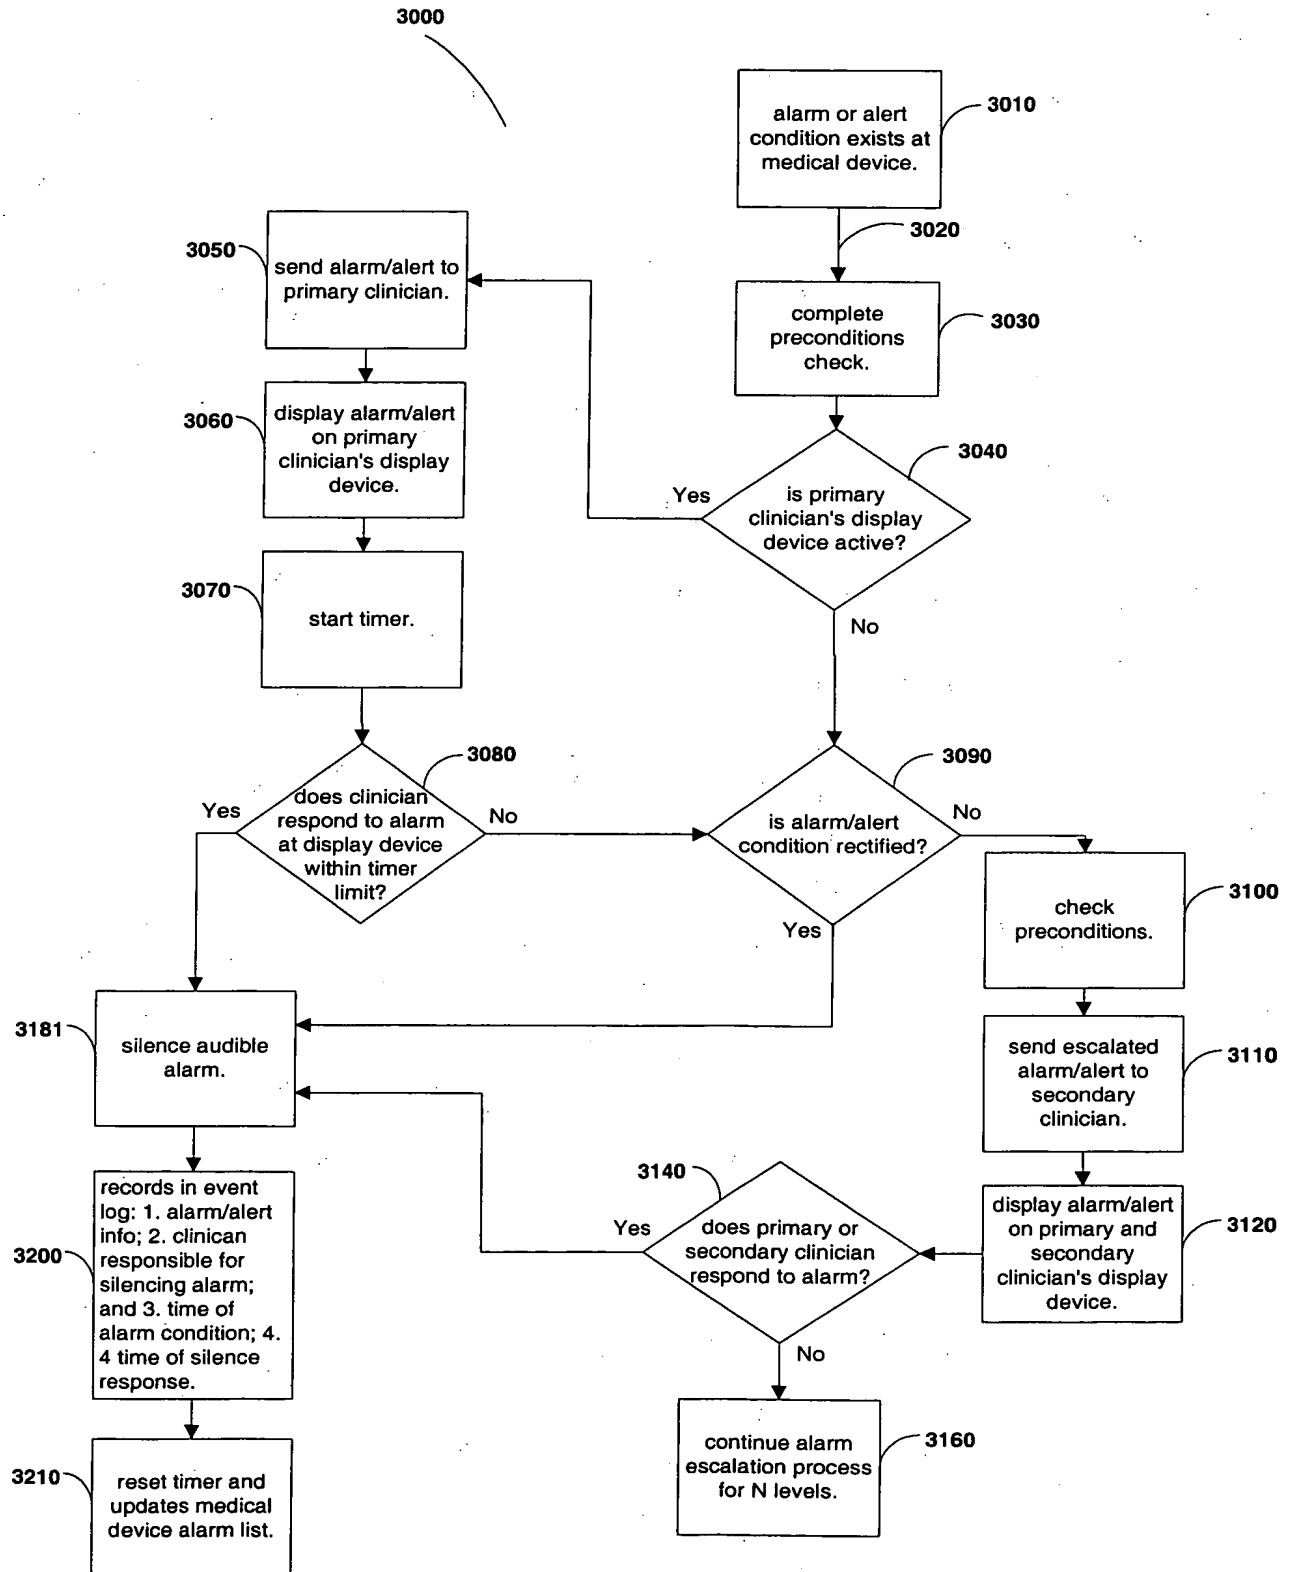


FIGURE 16a

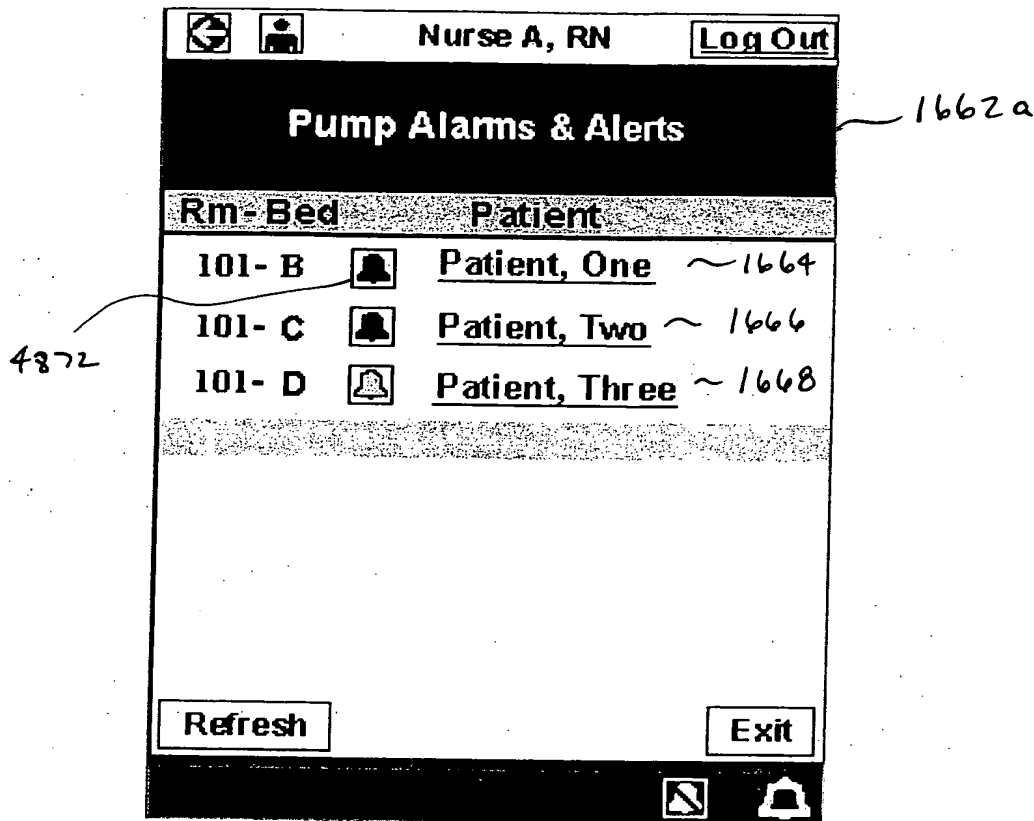


FIGURE 16b

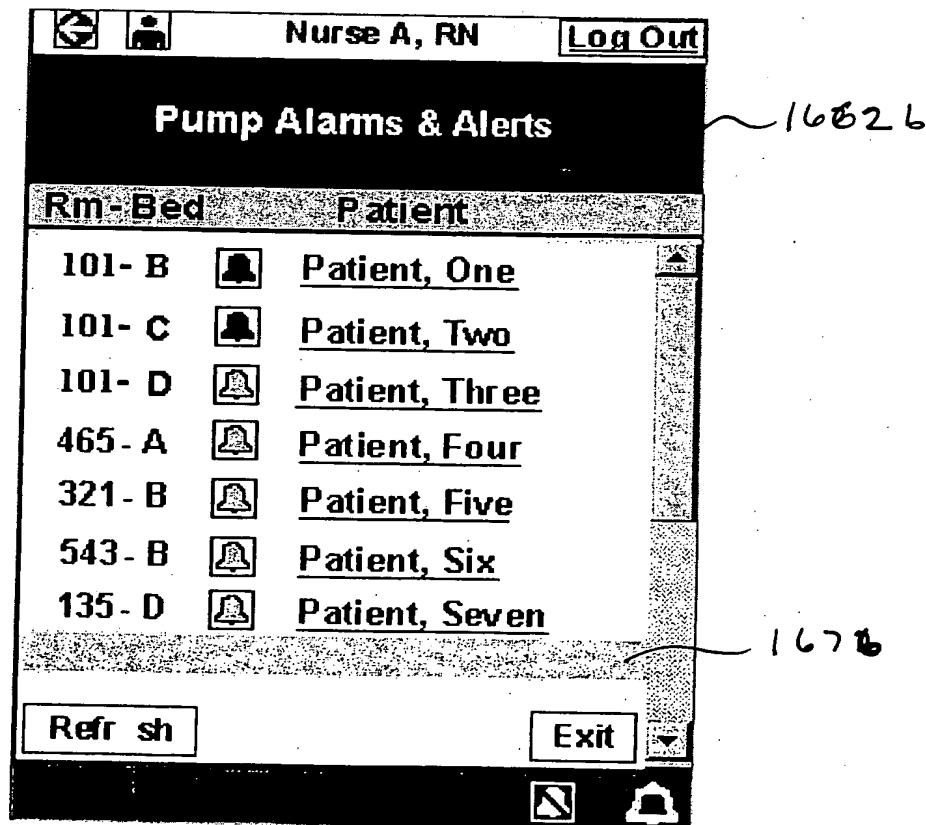


FIGURE 17

The screenshot shows a mobile application interface for 'Pump Alarms & Alerts'. At the top, there is a header bar with a navigation icon, a user icon, the text 'Nurse A, RN', and a 'Log Out' button. Below the header, the title 'Pump Alarms & Alerts' is displayed. The main content area is divided into sections: 'Rm - Bed' and 'Patient' with values '101- B' and 'Patient, One' respectively. Below this, there is a section for alarm messages, starting with '#1: Alarm message here' and the text 'Acef 1 g, in Dextrose, 5% 50 m'. At the bottom of the screen, there are 'Refresh' and 'Exit' buttons. A handwritten note '4819' points to the 'Refresh' button.

1765

4819

FIGURE 18

The screenshot shows a mobile application interface for 'Pump Alarms & Alerts', similar to Figure 17. It features the same header bar with 'Nurse A, RN' and a 'Log Out' button. The title 'Pump Alarms & Alerts' is present. The main content area shows 'Rm - Bed' as '101- B' and 'Patient' as 'Patient, One'. Below this, there are two identical alarm message sections, each starting with '#1: Alarm message here' and 'Acef 1 g, in Dextrose, 5% 50 m'. At the bottom, there are 'Refresh' and 'Exit' buttons. Handwritten notes '1867', '1878', and '1882' point to the title, the first alarm message, and the second alarm message respectively.

1867

1878

1882

FIGURE 19

Figure 19 shows a login screen for a "Patient Care System" at "General Hospital". The screen has a dark header with the system name and hospital name in white. Below the header, there are two input fields: "User Name" with the text "Nurse A" and "Password" with masked characters. A "Login" button is located below the password field. A reference numeral "1903" is positioned to the right of the header area.

FIGURE 20

Figure 20 shows the same login screen as Figure 19, but with a "Login failed" message and a prompt to "Check User Name or Password." The "User Name" and "Password" fields now have asterisks at the end, indicating they are required. A reference numeral "2005" is positioned to the right of the header area.



FIGURE 21

The screenshot shows a mobile application interface for a nurse. At the top, there is a header bar with the text "Nurse A, RN" and a "Log Out" button. Below this is a dark bar with the text "Select UNIT". The main area contains a list box with "Neurology ICU" selected, indicated by a checkmark. To the right of the list box is a right-pointing arrow button. A label "2105" points to the "Select UNIT" header, "4809" points to the arrow button, and "2107" points to the list box.


FIGURE 22




The screenshot shows a mobile application interface for selecting a work shift. At the top, there is a header bar with the text "Nurse A, RN" and a "Log Out" button. Below this is a dark bar with the text "Select WORK SHIFT". The main area contains two radio buttons: "Standard Shift" (selected) and "Customize Shift". Below the "Standard Shift" radio button is a list box with a right-pointing arrow button. A label "2255" points to the "Standard Shift" radio button, "2211" points to the "Select WORK SHIFT" header, "4809" points to the arrow button, and "2107" points to the list box. Below the "Customize Shift" radio button, there are two time selection fields: "Start: 18:30" and "End: 00:00".

FIGURE 23

  **Nurse A, RN** **Log Out**

My Patients **My Tasks**

Scan Patient: 

Rm - Bed		Patient
101 - B		Patient, One
101 - C		Patient, Two
101 - D		Patient, Three

Add More Patients

2313

2315


FIGURE 24

Nurse A, RN **Log Out**

Select PATIENTS

Rm - Bed	Patient
<input checked="" type="checkbox"/> 101 - B	<u>Patient, One</u>
<input checked="" type="checkbox"/> 101 - C	<u>Patient, Two</u>
<input checked="" type="checkbox"/> 101 - D	<u>Patient, Three</u>

Add patient for:



Find More Patients

2417

2419

FIGURE 25

Nurse A, RN **Log Out**

Patient, One -- 101-B 2521

Mini-Chart: Allergies (NKA)

Administer Meds/Infusions

STOP Infusion

RESUME Infusion

Titrate Infusion

Flow Rate History

Pump Status

Remove Patient from Shift

FIGURE 25a

Ninety-Three, James RN **Log Out**

Ninety-Nine, Douglas, Mr. (MDLOC1) 2521a

MDUnit1: MDRoom1 - MDBed1

Dr. Ninety, Susan

Mini-Chart: Allergies

Allergies & Ht/Wt **Med Hx**

Lab Results

Drug Allergy

Acetaminophen

General Allergy

Date Observed	Height	Weight
8-22 14:16	183.00 cm 72.05 in.	85.00 Kg 187.39 Lbs

Back

FIGURE 25b

Ninety-Three, James RN [Log Out](#)

Ninety-Nine, Douglas, Mr. (MDLOC1)
MDUnit1: MDRoom1 - MDBed1
Dr. Ninety, Susan

Mini-Chart Allergies (NKA)

Allergies & Ht/Wt **Med Hx**

Lab Results

All ☒ Scheduled ☐ PRN ☐

Look Back Period hours

Order

Acetaminophen Cap 500 MG
500 MG = 1 CAP
Oral
TID
Admin Date: 6-3 12:53
Patient Refused
[more...](#) ←

[Back](#)

2521b

FIGURE 25c

Ninety-Three, James RN [Log Out](#)

Ninety-Nine, Douglas, Mr. (MDLOC1)
MDUnit1: MDRoom1 - MDBed1
Dr. Ninety, Susan

Mini-Chart Allergies

Allergies & Ht/Wt **Med Hx**

Lab Results

Lab Test	Result	Range	H/L	Date
POTASSIUM	3.1	3.6 - 5 mmol/L	Normal	5/16/2003 9:00:00 AM

[Back](#)

2521c

FIGURE 26

	Time	Med	Last
<input checked="" type="checkbox"/>	11:30	MORPHINE SULFATE Continuous Infusion ⚠	12-9 2:00
<input type="checkbox"/>	13:30	Continuous Infusion (De SI NR	
<input type="checkbox"/>	15:30	Continuous Infusion (De SI NR	
<input type="checkbox"/>	17:30	Continuous Infusion (De SI NR ⚠	

2623

2625

FIGURE 26a

MA-Continuous Infusion
 Dextrose 5% w/Sodium Chloride 0.45%
 200 ML
 Route: Intravenous
 Flow Rate: 50 ML/H
 Estimated Admin. Period: 4 Hours

⚠ Warning: Wear Gloves

i Show Edubyte info here

RX not previously administered
 Start Time: 6-2 14:54
 End Time: 7-7 14:54

2627

2629

2631

2633

FIGURE 27a

The screenshot shows a web-based interface for a medical workflow. At the top, there is a header bar with a back arrow, a patient icon, the name 'Ninety-Three, James RN', and a 'Log Out' button. Below the header, the main content area has a dark background with white text. It starts with 'WORKFLOW INFUSION: STOP' in bold. Below that, it says 'Ninety-Six, Samuel, Mr. MDRoom1 - MDBed1'. There is a link for 'Mini-Chart Allergies'. A 'Scan Item:' field with a circular arrow icon is present. The infusion details are listed: 'Continuous Infusion', 'Dextrose Inj 20%', '500 ML', 'Route: Intravenous Flow Rate: 125 ML/H', and 'Estimated Administration Period: 4 Hours'. A status message 'Order has been D/C'd' is shown. At the bottom, there is a button labeled 'Back to Patient list'.

Ninety-Three, James RN [Log Out](#)

WORKFLOW INFUSION: STOP
Ninety-Six, Samuel, Mr. MDRoom1 - MDBed1
[Mini-Chart Allergies](#)

Scan Item:

Continuous Infusion
Dextrose Inj 20%
500 ML
Route: Intravenous Flow Rate: 125 ML/H
Estimated Administration Period: 4 Hours

Order has been D/C'd

[Back to Patient list](#)

2727a

FIGURE 27b

This screenshot is similar to Figure 27a but includes an additional step for stopping the infusion. It shows the same header and patient information. The infusion details are the same. Below the status message, there is a prompt 'Please select a reason for Stop Infusion' followed by a dropdown menu with 'Discontinue order in system' selected. Below that is a 'Stop Time' section with three dropdown menus for date and time: '06/18/2003', '15', and '23'. At the bottom, there is a 'Cancel' button with a circular arrow icon and a 'Back to Patient list' button.

Ninety-Three, James RN [Log Out](#)

WORKFLOW INFUSION: STOP
Ninety-Six, Samuel, Mr. MDRoom1 - MDBed1
[Mini-Chart Allergies](#)

Continuous Infusion
Dextrose Inj 20%
500 ML
Route: Intravenous Flow Rate: 125 ML/H
Estimated Administration Period: 4 Hours

Please select a reason for Stop Infusion

Stop Time[M/D/Y HH:MM]

Cancel

[Back to Patient list](#)

2727b

FIGURE 27c

A screenshot of a medical workflow interface. At the top, a header bar contains a back arrow, a user icon, the text "Ninety-Three, James RN", and a "Log Out" button. Below the header, the main content area has a dark background with white text. It starts with "WORKFLOW INFUSION: RESUME" in a bold box. Below this, it says "Ninetyfour-Pointfive, Fred , Mr." and "MDRoom1 - MDBed4". A link "Mini-Chart Allergies (Not Specified)" is visible. There is a "Scan Item:" label followed by a text input field and a circular arrow icon. The main text area lists: "Continuous Infusion", "Dextrose Inj 20%", "500 ML", "Route: Intravenous Flow Rate: 125 ML/H", and "Estimated Administration Period: 4 Hours". Below this, it says "Stopped w/o Order". At the bottom, there is a button labeled "Back to Patient list".

2727c

FIGURE 27d

A screenshot of a medical workflow interface, similar to Figure 27c. It has the same header bar with "Ninety-Three, James RN" and "Log Out". The main content area has a dark background with white text. It starts with "WORKFLOW INFUSION: RESUME" in a bold box. Below this, it says "Ninetyfour-Pointfive, Fred , Mr." and "MDRoom1 - MDBed4". A link "Mini-Chart Allergies (Not Specified)" is visible. The main text area lists: "Continuous Infusion", "Dextrose Inj 20%", "500 ML", "Route: Intravenous Flow Rate: 125 ML/H", and "Estimated Administration Period: 4 Hours". Below this, it says "Stopped w/o Order" and "Please select a reason for Resume Infusion". There is a dropdown menu with "Site re-established" selected. At the bottom, there is a "Cancel" button with a circular arrow icon and a button labeled "Back to Patient list".

2727d

4809

FIGURE 28

Nurse A, RN Log Out

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

< 10:19 - 12:19 >

SCHED 13

	Time	Med	Last
<input checked="" type="checkbox"/>	13:30	MORPHINE SULFATE Continuous Infusion	12:00
<input type="checkbox"/>	13:30	Continuous Infusion (De SI	
<input type="checkbox"/>	15:30	Continuous Infusion (De SI	
<input type="checkbox"/>	17:30	Continuous Infusion (De	

4837

2835

2839

FIGURE 29

Nurse A, RN Log Out

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

☒ Missed Medication

Please select a reason for LATE:

☐ Adjust schedule for:

MORPHINE SULFATE
Continuous Infusion
60 MG = 30 ML
Route: Injection
Flow Rate: 30 ML/H
Estimated Admin. Period: 1 Hour

4837

2941

2943

2945

FIGURE 30

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

Missed Medication
Please select a reason for LATE

Patient unavailable at sched. time

Not Required

Cycle Count

Insufficient Stock

Re-open drawer

Maintain Admin Test

Already have item

Item Unavailable

Refused

3047

3045

FIGURE 31

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

< 10:19 - 12:19 >

SCHED 13

	Time	Med	Last
<input type="checkbox"/>	13:30	MORPHINE SULFATE Continuous Infusion	12-9 2:00
	NR		
<input type="checkbox"/>	13:30	Continuous Infusion (De SI	
	NR		
<input type="checkbox"/>	15:30	Continuous Infusion (De SI	
	NR		
<input type="checkbox"/>	17:30	C ntinuous Infusion (De	
	NR		

4857

3135

2839

FIGURE 32

Nurse A, RN **Log Out**

SCHD 13

	Time	Med	Last
<input checked="" type="checkbox"/>	11:30	MORPHINE SULFATE Continuous Infusion ⚠	12/9 2:00
<input type="checkbox"/>	13:30 NR	Continuous Infusion (De SI	
<input type="checkbox"/>	15:30 NR	Continuous Infusion (De SI	
<input type="checkbox"/>	17:30 NR	Continuous Infusion (De ⚠	

Get Items

Handwritten labels: 3235 points to the top right area; 3225 points to the first medication row; 3249 points to the 'Get Items' button.

FIGURE 33

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

Scan Depot:

Search Items

Item	DepotUnit	Qty
Morphine Sulfate Inj 2 MG/ML QA	in other units	
Morphine Sulfate Inj 2 MG/ML QA	in other units	

Skip Scan Depot

Handwritten labels: 3353 points to the 'Scan Depot' field; 3355 points to the 'Skip Scan Depot' button; 3351 points to the right side of the interface.

FIGURE 34

3467

3465

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

Rx Scan Item: **➔**

MORPHINE SULFATE
Continuous Infusion
60 MG = 30 ML
Route: Injection
Flow Rate: 30 ML/H
Estimated Admin. Period: 1 Hour

Quantity: ML(s)

Get: 30 ML

Warning: Wear Gloves

Show Edubyte info here

FIGURE 35

3569

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart: Allergies (NKA)

Scan Depot: **➔**

Scan code is invalid.

Search Items

Item	DepotUnit	Qty
Morphine Sulfate Inj 2 MG/ML QA	in other units	
Morphine Sulfate Inj 2 MG/ML QA	in other units	

Skip Scan Depot

FIGURE 36

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart Allergies (NKA)

Scan Patient:

If cannot admin, select a reason:

Not Req Due to Monitoring Result

Patient Unavailable

Refused

Waste/Return

3657

3659

3661

3663

FIGURE 37

Nurse, C RN **Log Out**

Patient Three, Mr. 100-C

Mini-Chart Allergies!

Verify Route, Line & Site

Rx Sodium Chloride 0.9% Continuous Infusion

Rx Sodium Chloride 0.9% 1000 ML

Route: Intravenous Flow Rate: 50 ML/H

Estimated Administration Period: 20 Hours

Please hang the bag, program the pump and record the following information but DO NOT start the pump channel until instructed:

Route:

Line:

Site:

Compar Route

3771

3773

3775

3777

3778

4817

FIGURE 38

Nurse, C RN Log Out

Patient: Three Mr. 100 C
Mini-Chart Allergies!

Select Pump Channel Mode

Rx Sodium Chloride 0.9%
Continuous Infusion
Rx Sodium Chloride 0.9%
1000 ML
Route: Intravenous Flow Rate: 50 ML/H
Estimated Administration Period: 20 Hours

Select Pump Channel Mode:

Primary ☒ 3884 Pingback ☐ 3883

3881

3882

FIGURE 38a

Nurse, C RN Log Out

Patient: Three Mr. 100 C
Mini-Chart Allergies!

Scan Pump Channel

Rx Sodium Chloride 0.9%
Continuous Infusion
Rx Sodium Chloride 0.9%
1000 ML
Route: Intravenous Flow Rate: 50 ML/H
Estimated Administration Period: 20 Hours

Scan Pump Channel 4809

3885

FIGURE 39

Nurse, C RN Log Out

Patient, Three, Mr.
 1 West: 100 - C
 MD1, Test

Pharm & Pump Comparison

Continuous Infusion Rx Sodium Chloride 0.9% 1000 ML Route:
 Intravenous Flow Rate: 50 mL/H Estimated Administration
 Period: 20 Hours

Program the Pump Channel and:

- > If this is a PRIMARY –
 Click COMPARE below Now and
 wait until instructed to start pump channel.
- > If this is a PIGGYBACK –
 Press the "Start" key on the
 pump Now, then Click COMPARE.

If Piggyback Infusion, ensure PRIMARY is placed LOWER THAN
 than PIGGYBACK and that PIGGYBACK roller clamp is OPEN.

Compare

3986

4817

FIGURE 39a

Nurse A, RN Log Out

Patient, One
 Rm - Bed 101-B
 Dr. One (111) 111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g, in Dextrose, 5 % 50 mL
 run at 100 mL/hr

	Pharm Label	=	Pump Settings
Rate	100 mL/hr		100 mL/hr

Comparison MATCHES.
 Press "Start" key on pump.

OK

3987

FIGURE 40

U.S. Patent Application of T. Simpson, et al.
 Mailed: December 30, 2003
 Atty Docket No. EIS-5909H (1417GP984)
 Sheet 31 of 58

Nurse A, RN **Log Out**

Patient, One
Rm - Bed 101-B
Dr. One (111)111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g, in Dextrose, 5 % 50 mL
 run at 100 mL/hr

	Pharm Label	Pump Settings
Rate	100 mL/hr	50 mL/hr

Please Verify with PHYSICIAN Order.
 Then to accept the mismatch, press "Start"
 key on pump and then click "OK" below.
 You can also reprogram the pump and
 then click "Compare again".

OK **Compare again**

4087

4825

4817

FIGURE 41

Nurse A, RN **Log Out**

Patient, One
Rm - Bed 101-B
Dr. One (111)111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g, in Dextrose, 5 % 50 mL
 run at 100 mL/hr

	Pharm Label	Pump Settings
Rate	100 mL/hr	? mL/hr

Cannot compare.
 Press "Rate" key and COMPARE.

COMPARE

4187

4817

FIGURE 42

Nurse A, RN Log Out

Patient, One
Rm - Bed 101-B
Dr. One (111)111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g, in Dextrose, 5 % 50 mL
run at 100 mL/hr

	Pharm Label	? Pump Settings
Rate	100 mL/hr	? mL/hr

Cannot compare. Press "Start" key on pump and click COMPARE, to retry comparison.

COMPARE

Baxter

FIGURE 43

Nurse A, RN Log Out

Patient, One
Rm - Bed 101-B
Dr. One (111)111-1111 ext. 1

Pump Status

Ancel 1 g, in Dextrose, 5 % 50 mL
run at 100 mL/hr

Rate	60 mL/h
Volume Infused	5 mL
Volume Remaining	45 mL
Time Remaining	45 min.

*NOTE: Pump Override Accepted

Refr sh Exit

Baxter

FIGURE 44

Nurse A, RN **Log Out**

Patient, One
Rm - Bed 101-B
Dr. One (111)111-1111 ext. 1

Flow Rate History

Ancef 1 g, in Dextrose, 5 % 50 mL
run at 100 mL/hr

60 mL/h	@	10:55 AM	3/13
70 mL/h	@	10:55 AM	3/13
80 mL/h	@	10:54 AM	3/13

Refresh **Exit**

4493

FIGURE 45a

Nurse A, RN **Log Out**

Communication Loss Alert
 for the following Patients

Rm - Bed	Patient
101- B	<input checked="" type="checkbox"/> <u>Patient, One</u>
101- C	<input checked="" type="checkbox"/> <u>Patient, Two</u>
101- D	<input checked="" type="checkbox"/> <u>Patient, Three</u>

Trouble Shooting Tips:
 If a Yellow light is flashing on the WIRELESS MODULE and it is beeping, the system may be down. Call IT or Biomed.
 - OR -
 Plug in and turn on all pumps.
 If that does not resolve the problem, call IT or Biomed.

4501

FIGURE 45b

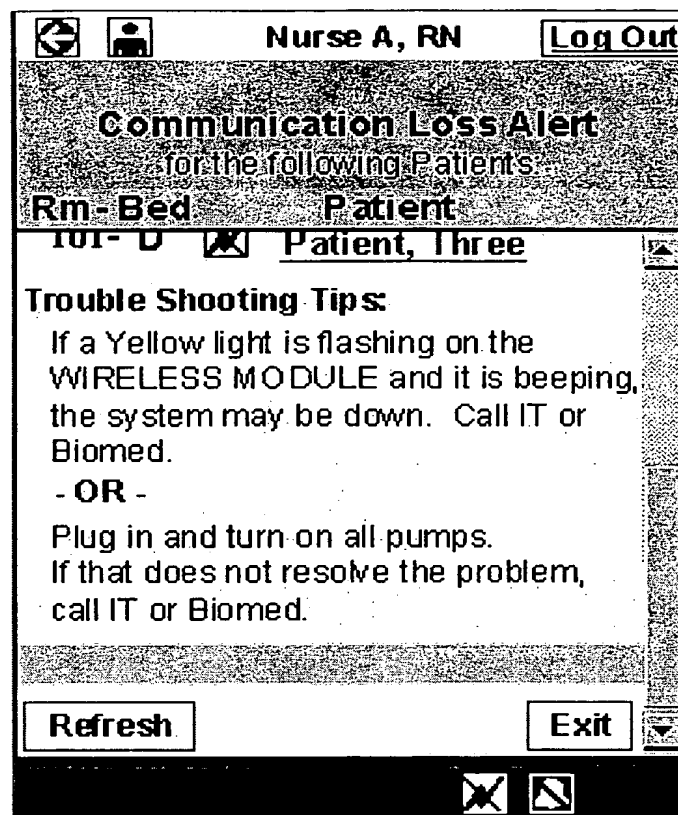


FIGURE 46

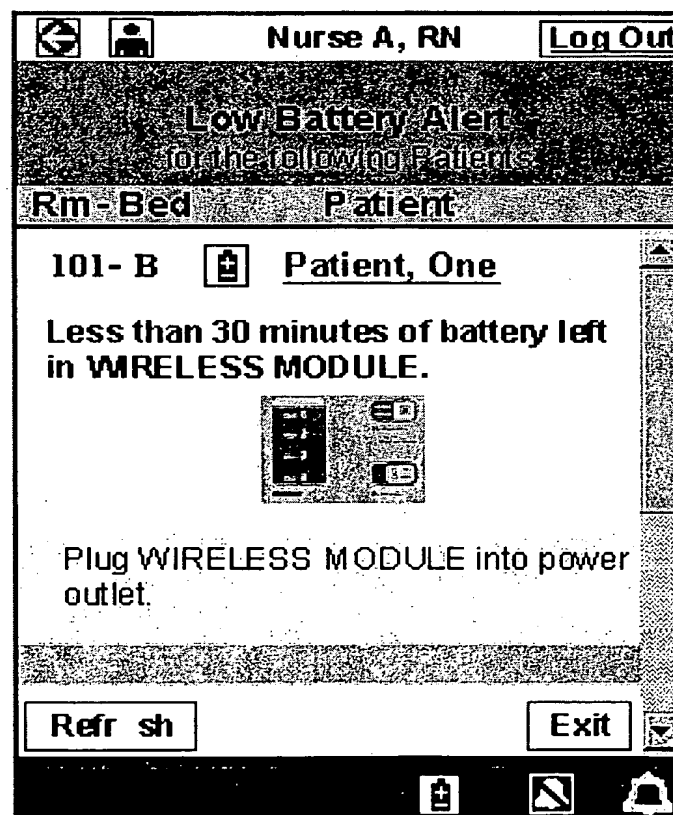


FIGURE 47

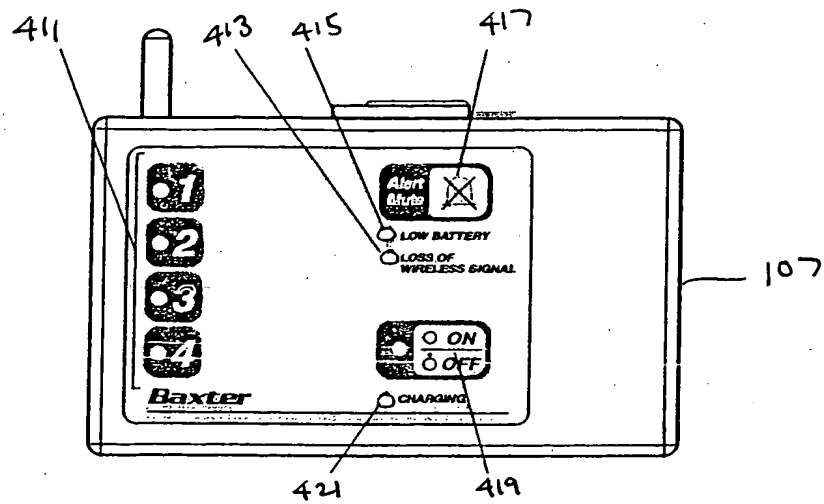


FIGURE 48




















Icon		Icon	
	4801		4805
	4803		4823
	4805		4825
	4807		4827
	4809		4872
	4811		
	4813		
	4815		
	4817		4874
			4833
	4819		
	4821		4835

FIGURE 49

Nurse A, RN **Log Out**

Patient, One - 101-B

Mini-Chart Allergies (NKA)

Record Admin Result

Please select Admin Result:

MORPHINE SULFATE
Continuous Infusion
60 MG = 30 ML
Route: Injection
Flow Rate: 30 ML/H
Estimated Admin. Period: 1 Hour

4937

FIGURE 50

	Time	Med	Last
<input type="checkbox"/>	14:39	Digoxin Tab 0.125	
	NR	MG 0.125 MG = 1	
		TAB Oral QD q 1	
		MP ←	

5001

FIGURE 50a

Ninety-Three, James RN **Log Out**

Ninety-Six, Samuel, Mr. MDRoom1 - MDBed1

Mini-Chart Allergies (NKA)

Monitoring Parameters

Blood Pressure

Mm/Hg.

Supine

Save

- Back -

5003

FIGURE 51

The screenshot shows a medical software interface. At the top, there is a header bar with a user icon, the text "Ninety-Three, James RN", and a "Log Out" button. Below the header, a patient selection bar displays "Eightytwo, Anthony, MDRoom1 - MDDefaultBed". The main content area is titled "Mini-Chart Allergies" and contains the following text: "ACETAMINOPHEN/CODEINE #4", "Acetaminophen w/ Codeine Tab", "300-60 MG 60 MG = 1 TAB Oral", and "QID". Below this, it says "Drawer 1, Bin 05". A section for medication counting follows, with the text "Count before the removal of medication (first count)" and "Qty on hand:". There is an input field for the quantity, followed by the text "TAB(s)". Below the input field is the label "Count". At the bottom of the interface are two buttons: "Back to Patient List" and "Re-open drawer".

Ninety-Three, James RN Log Out

Eightytwo, Anthony, MDRoom1 - MDDefaultBed

Mini-Chart Allergies

ACETAMINOPHEN/CODEINE #4
Acetaminophen w/ Codeine Tab
300-60 MG 60 MG = 1 TAB Oral
QID

Drawer 1, Bin 05

Count before the removal of
medication (first count)
Qty on hand:

TAB(s)

Count

Back to Patient List
Re-open drawer

5101

FIGURE 52

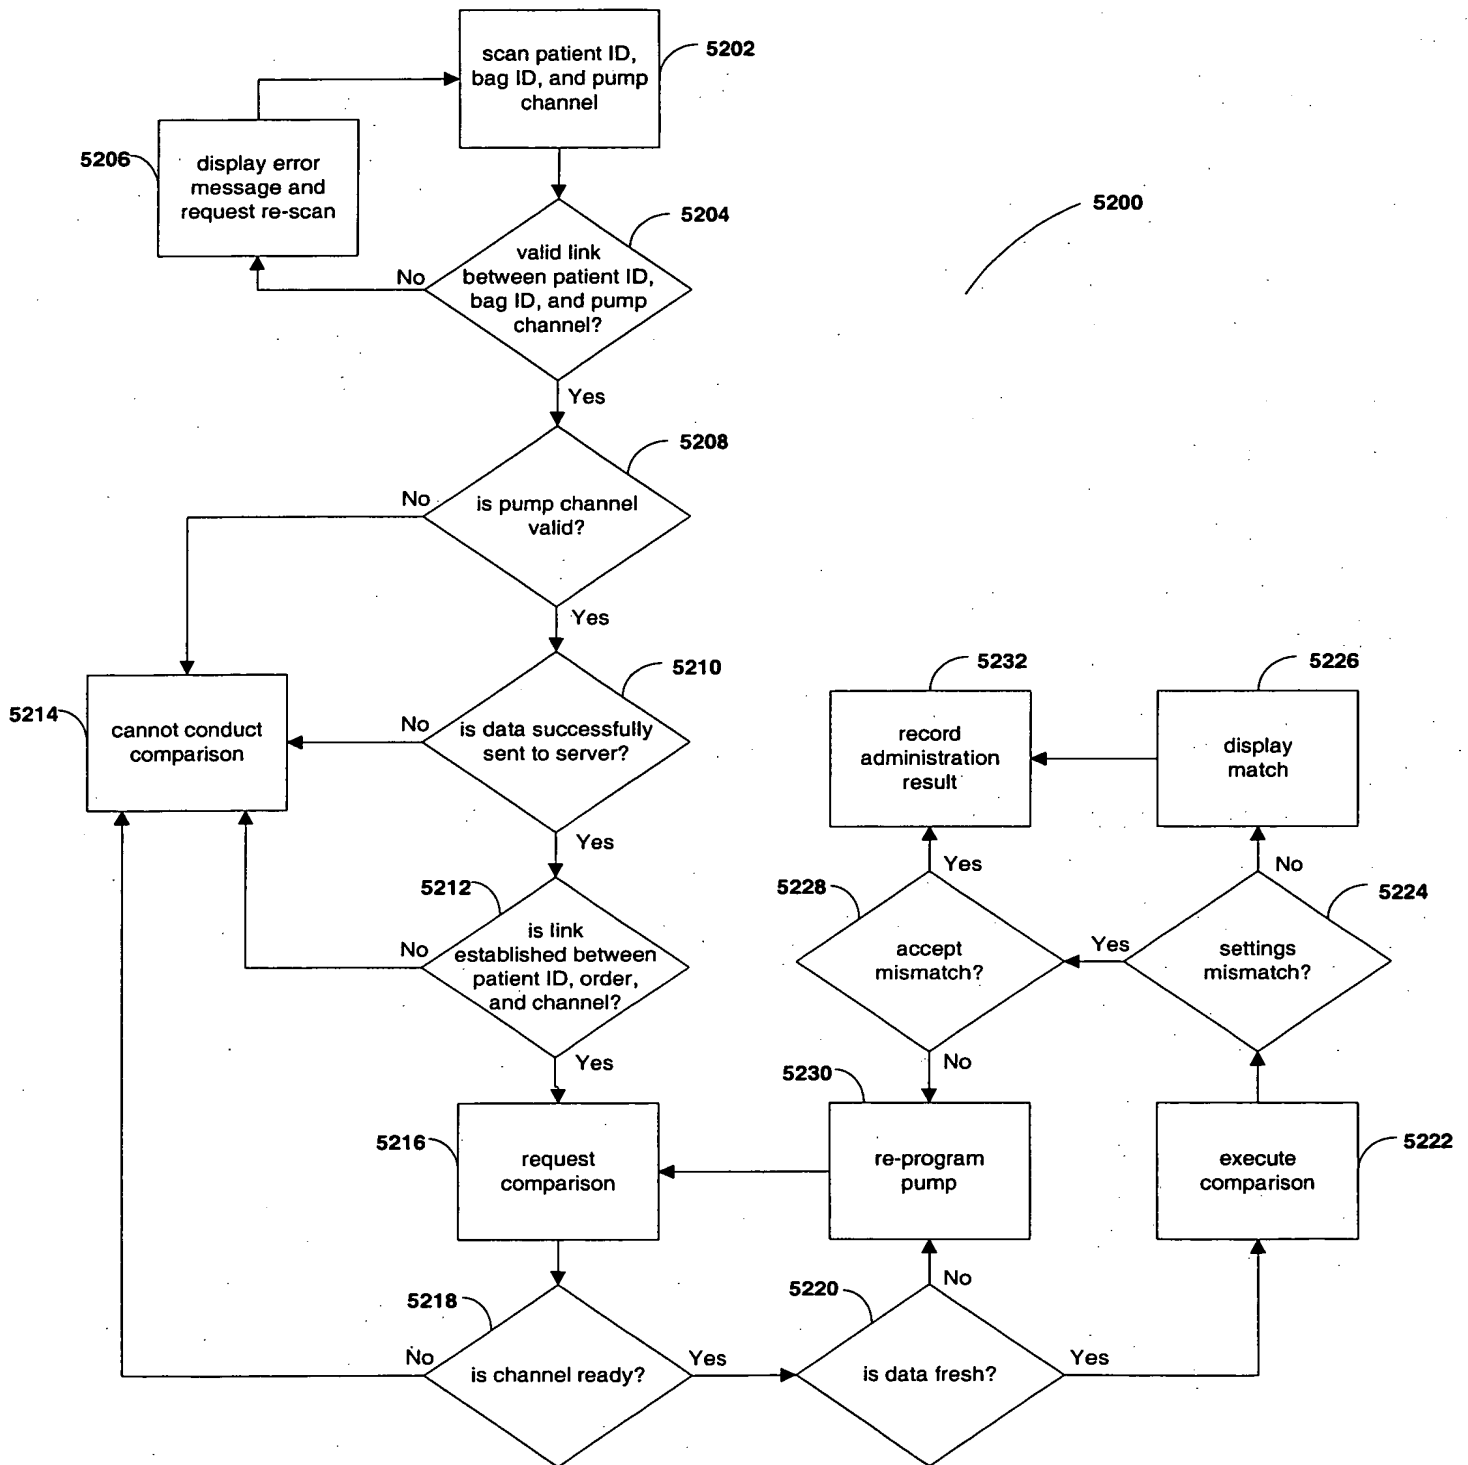
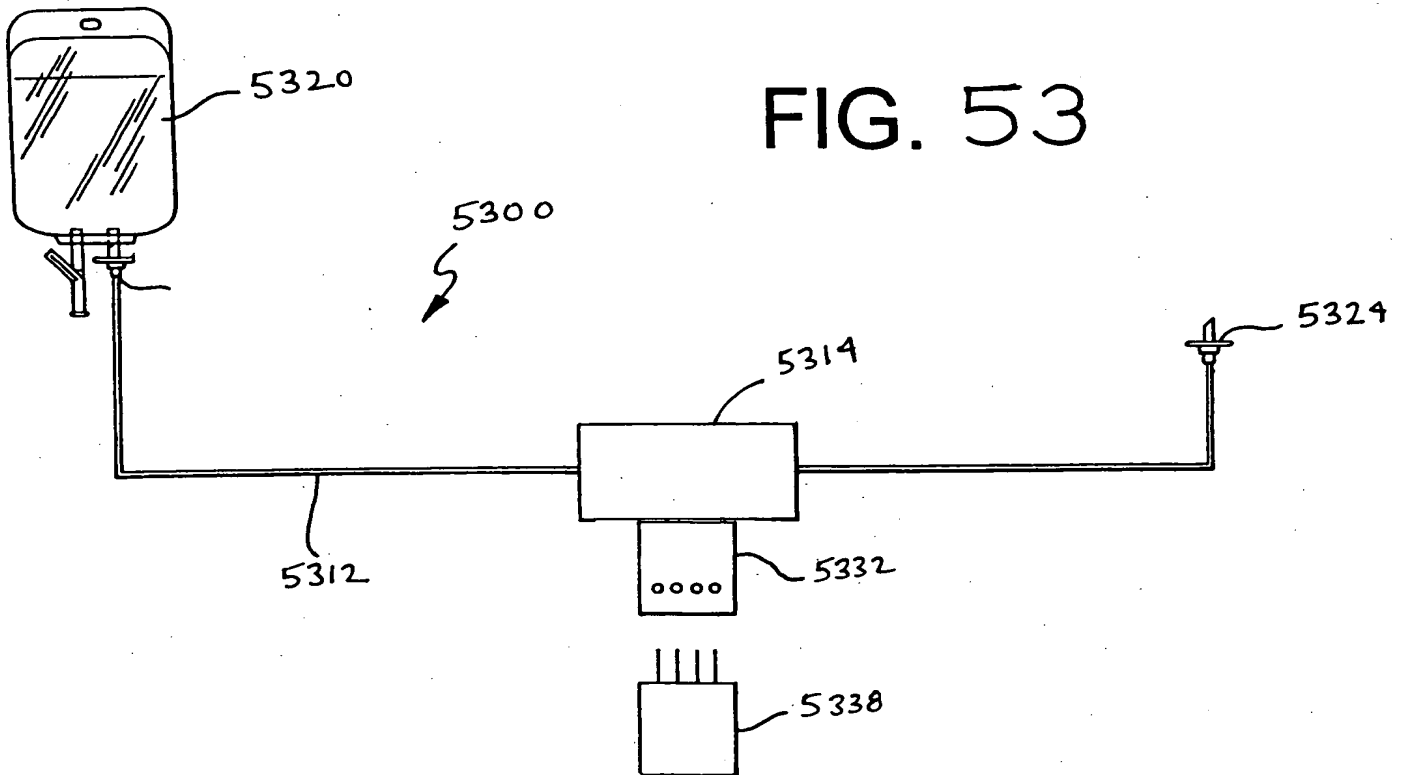


FIG. 53



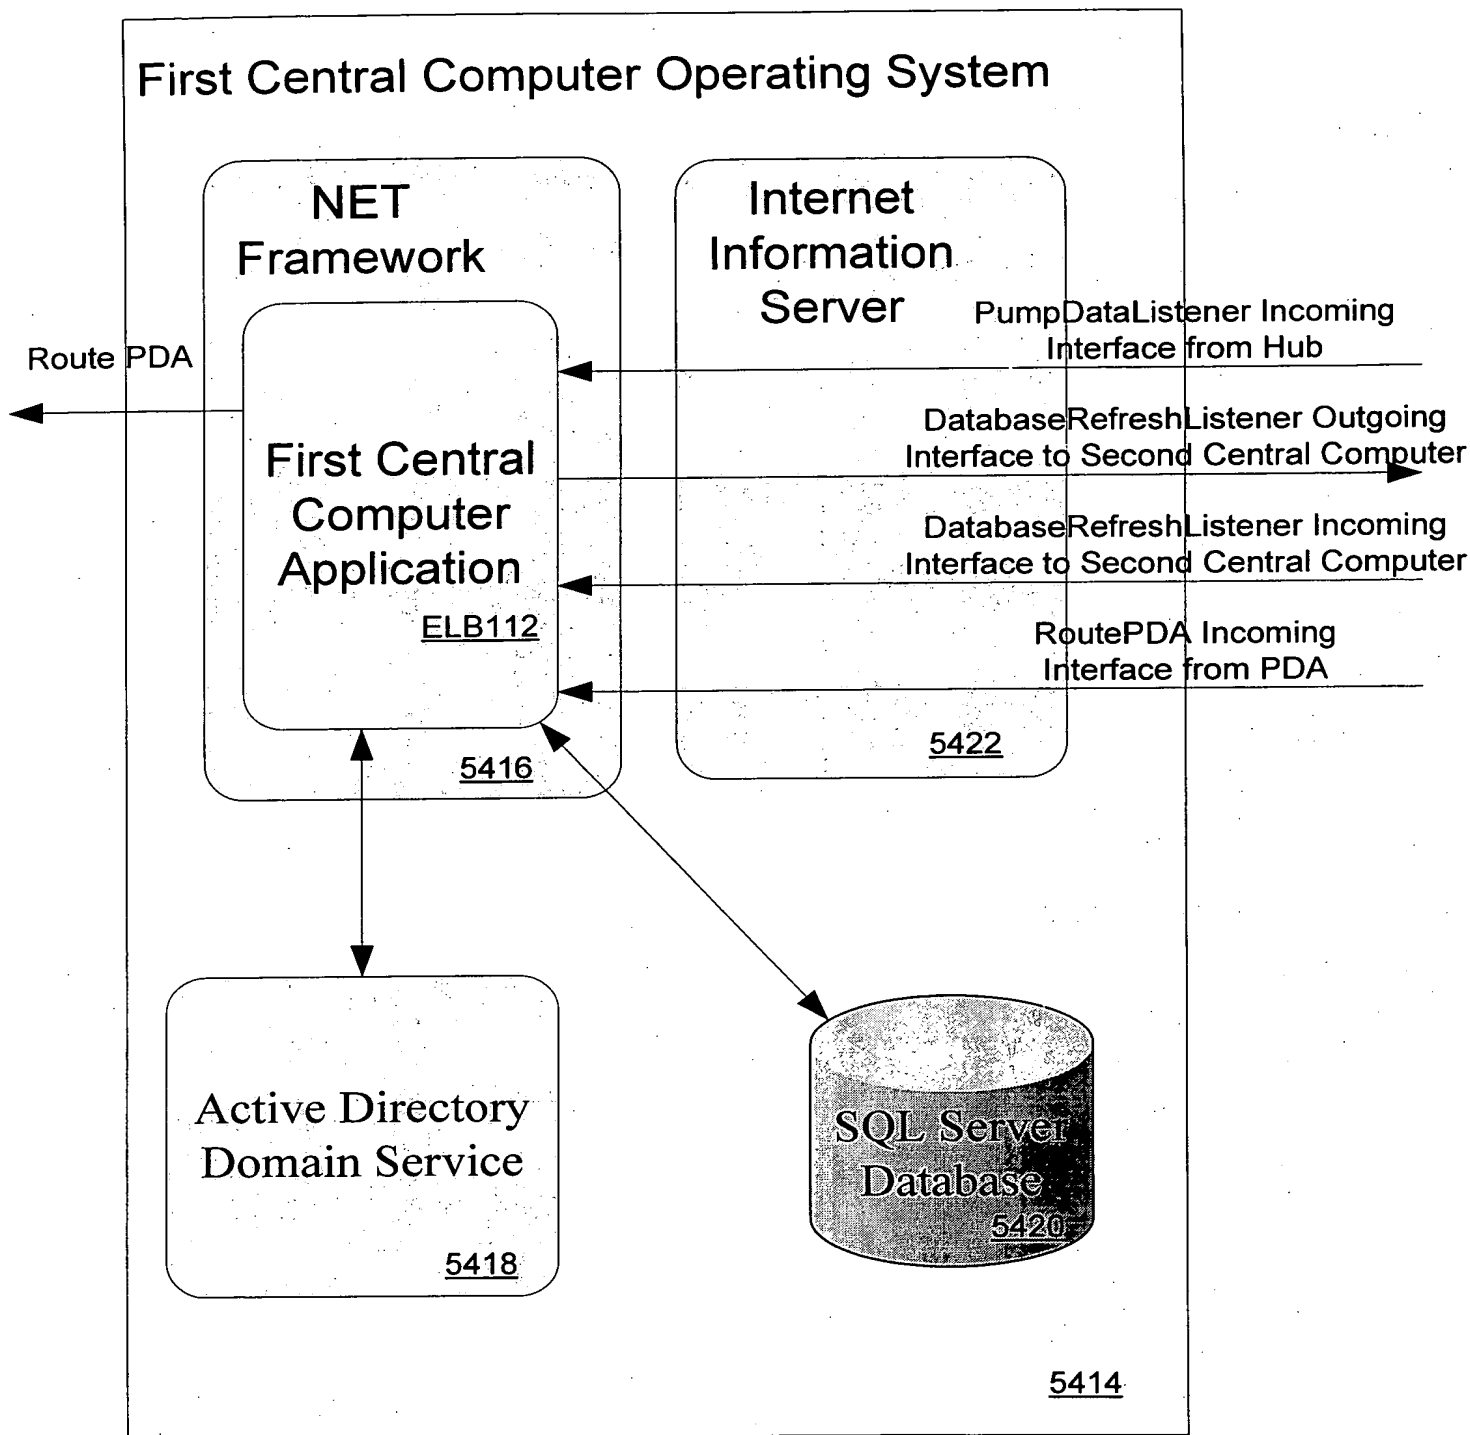


FIGURE 54

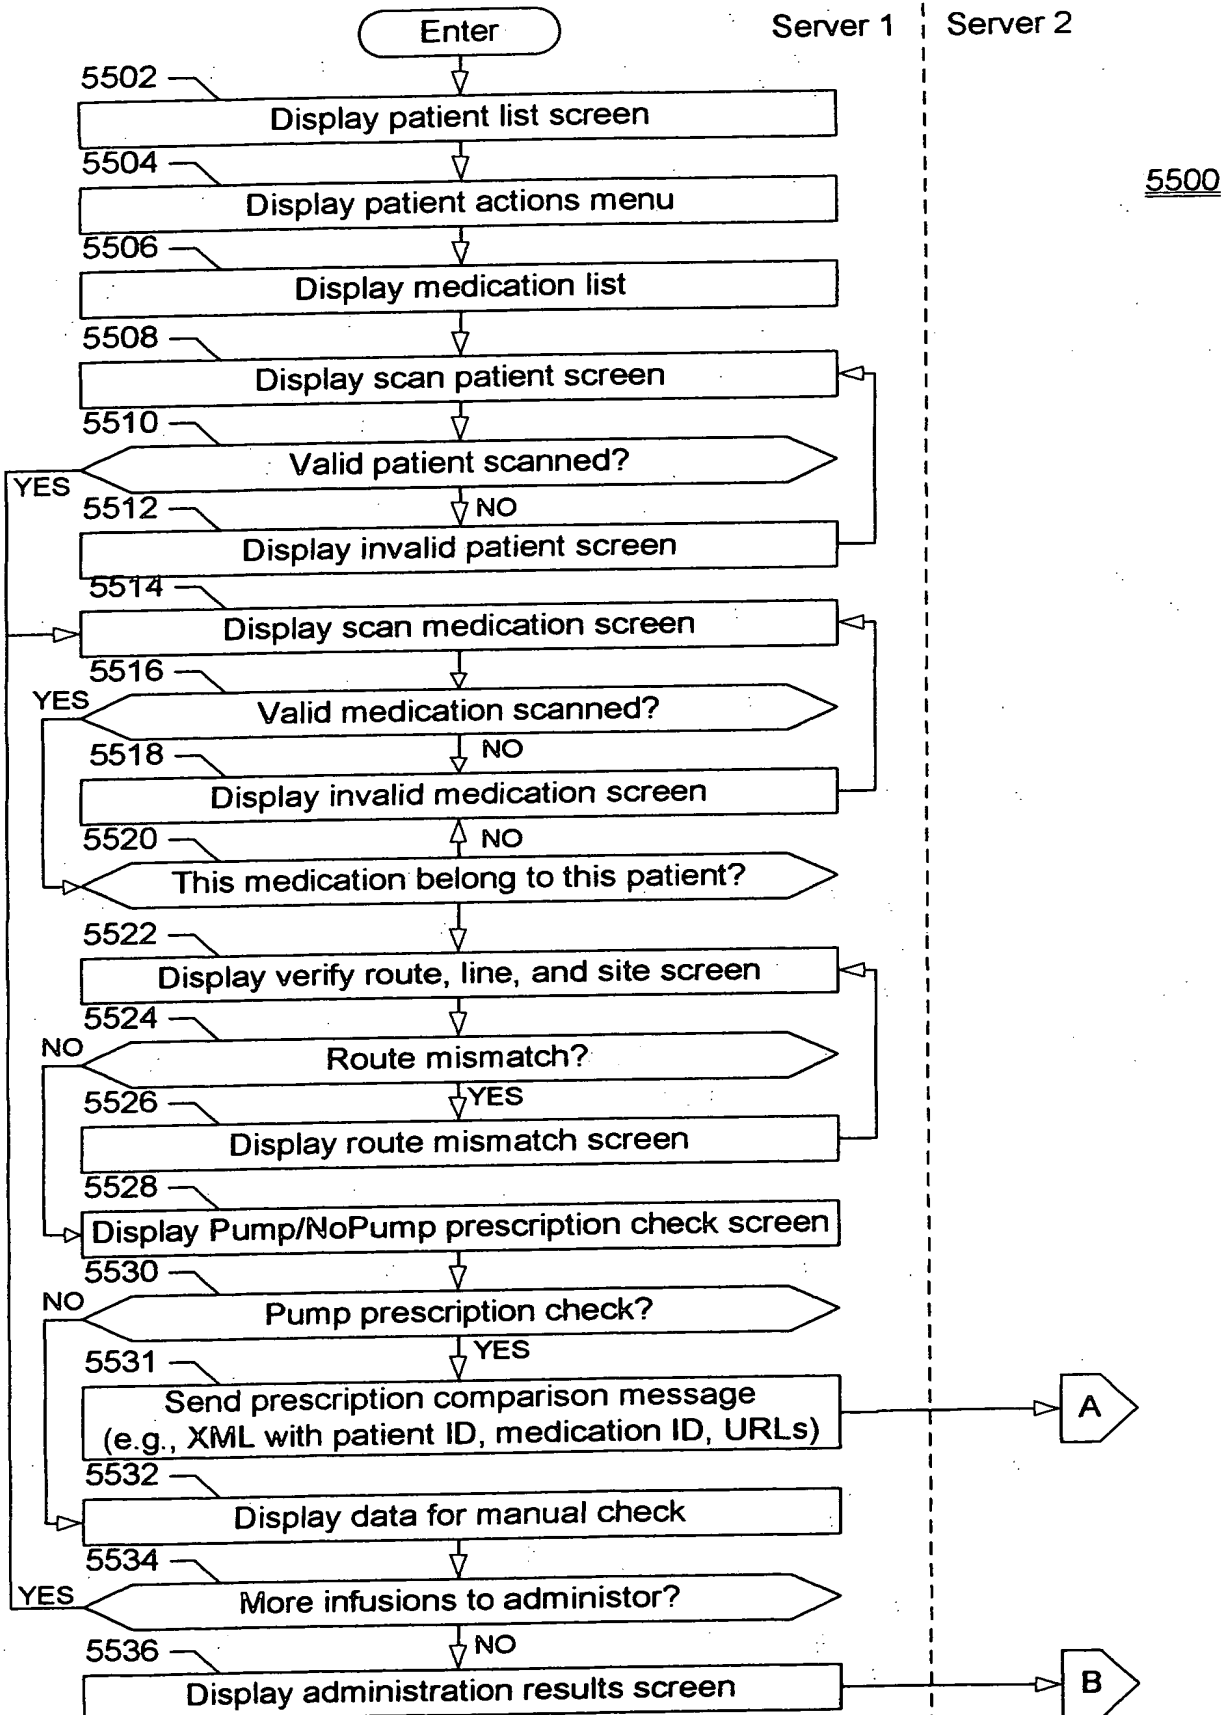
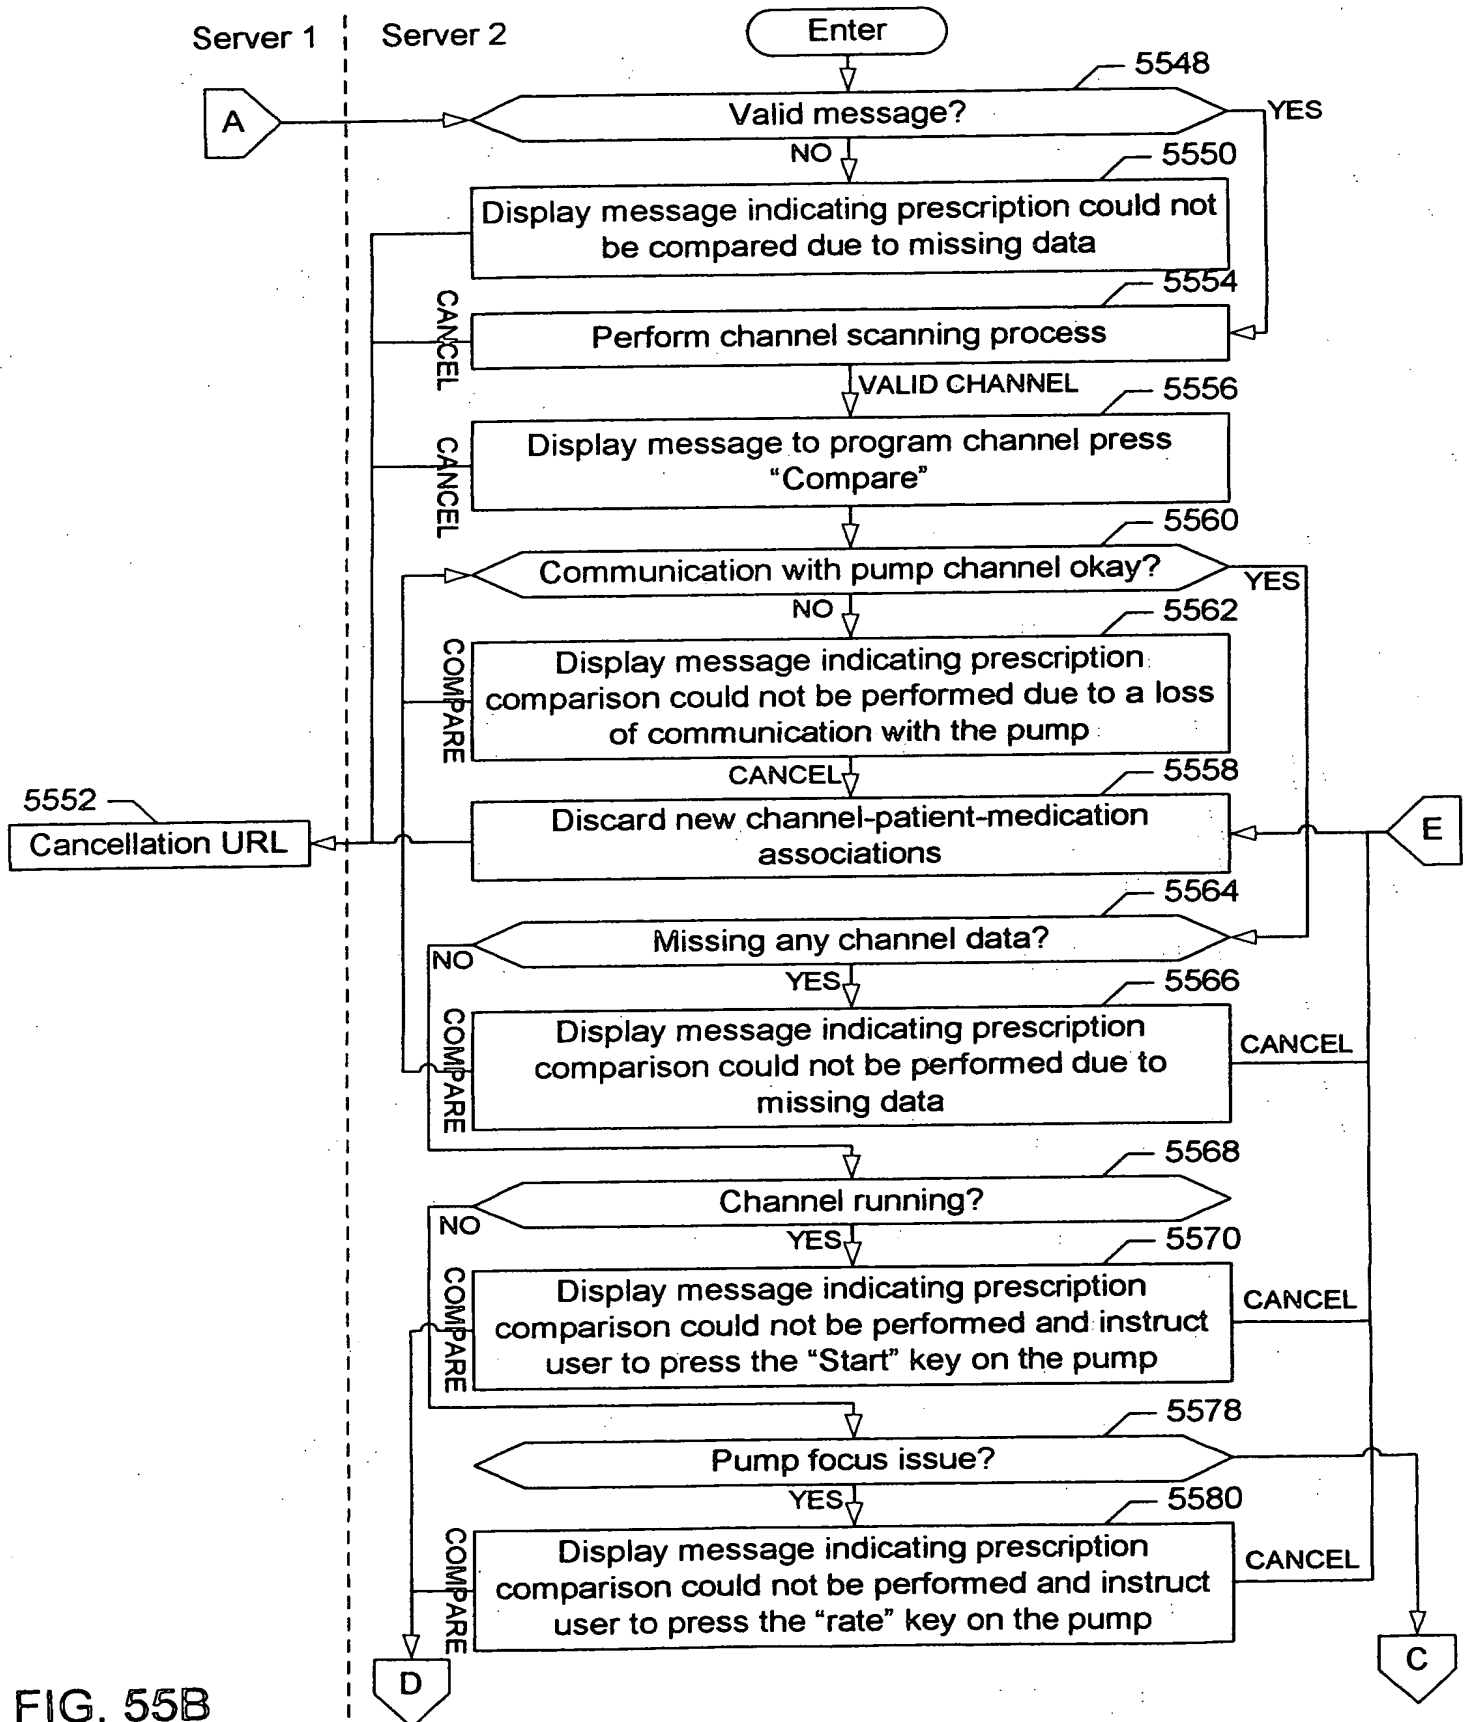


FIG. 55A



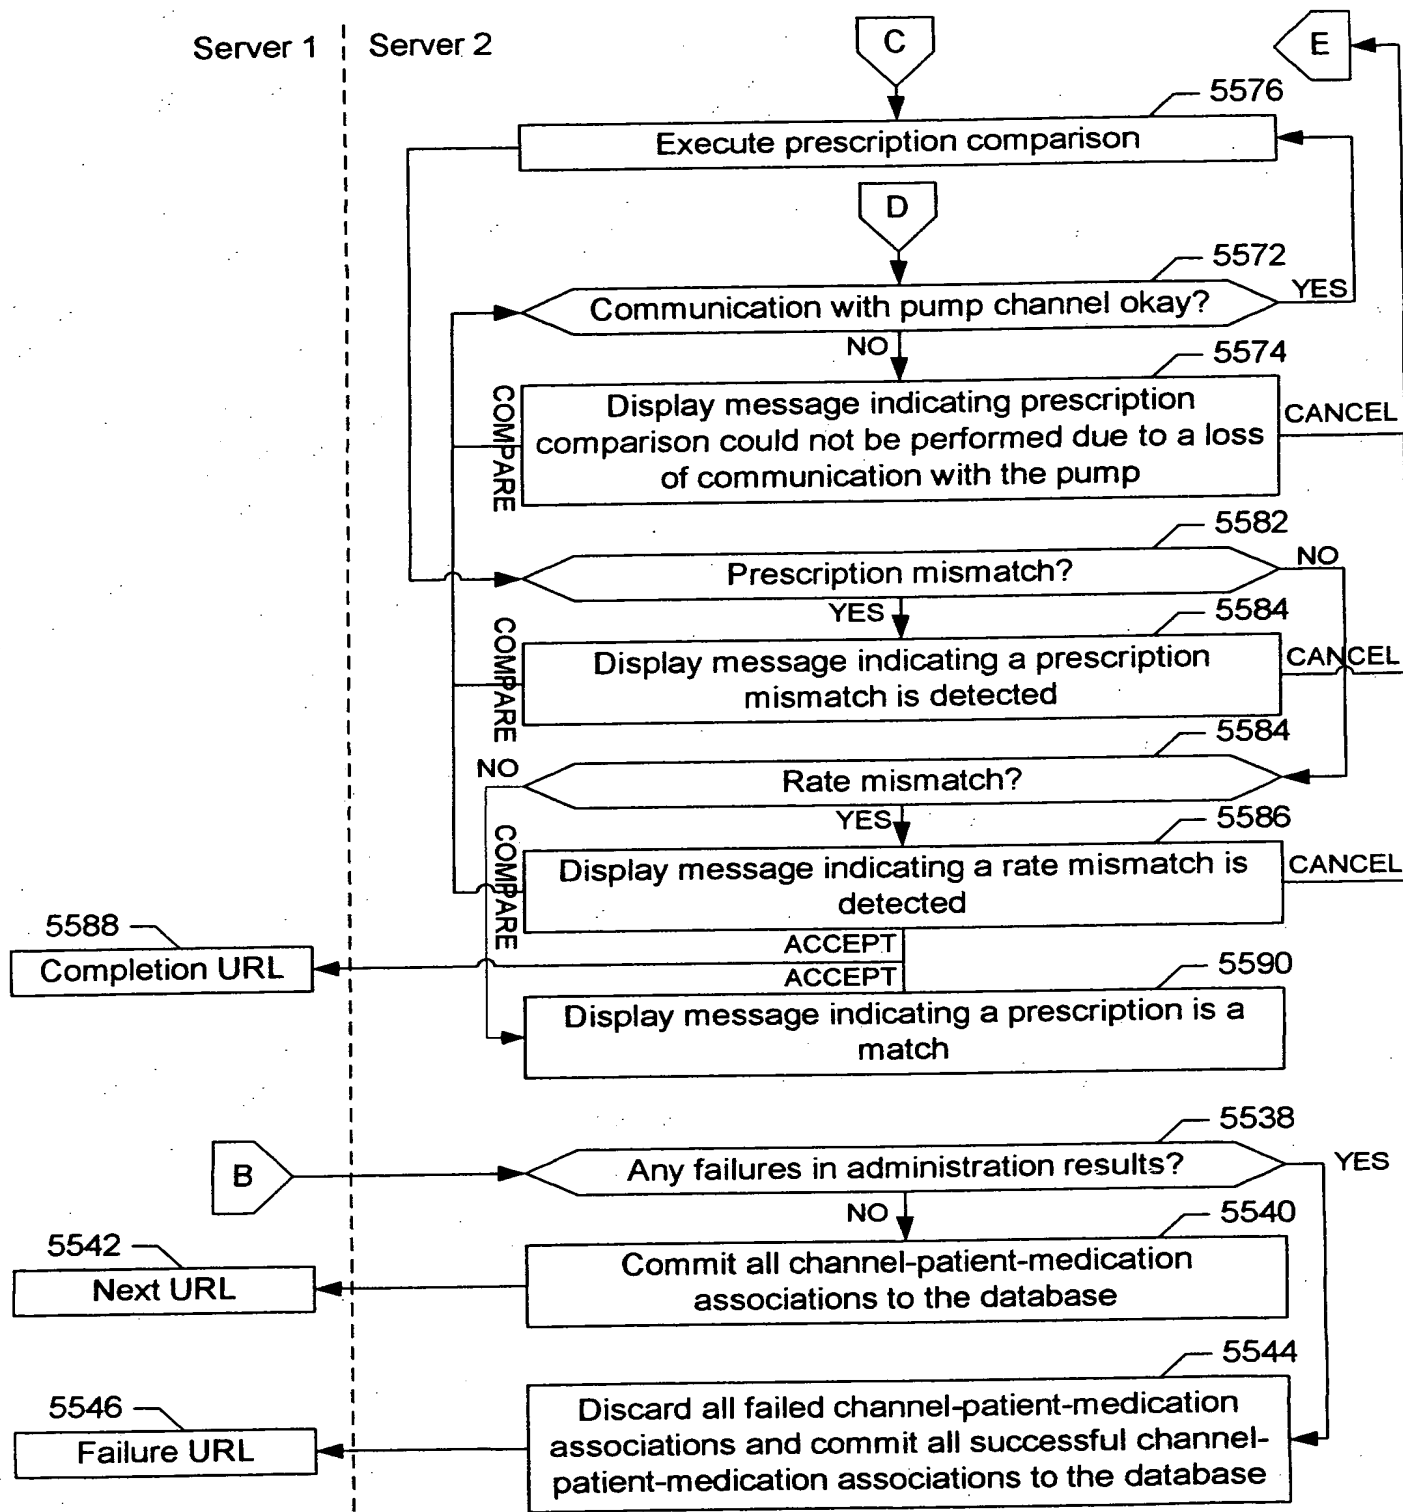


FIG. 55C

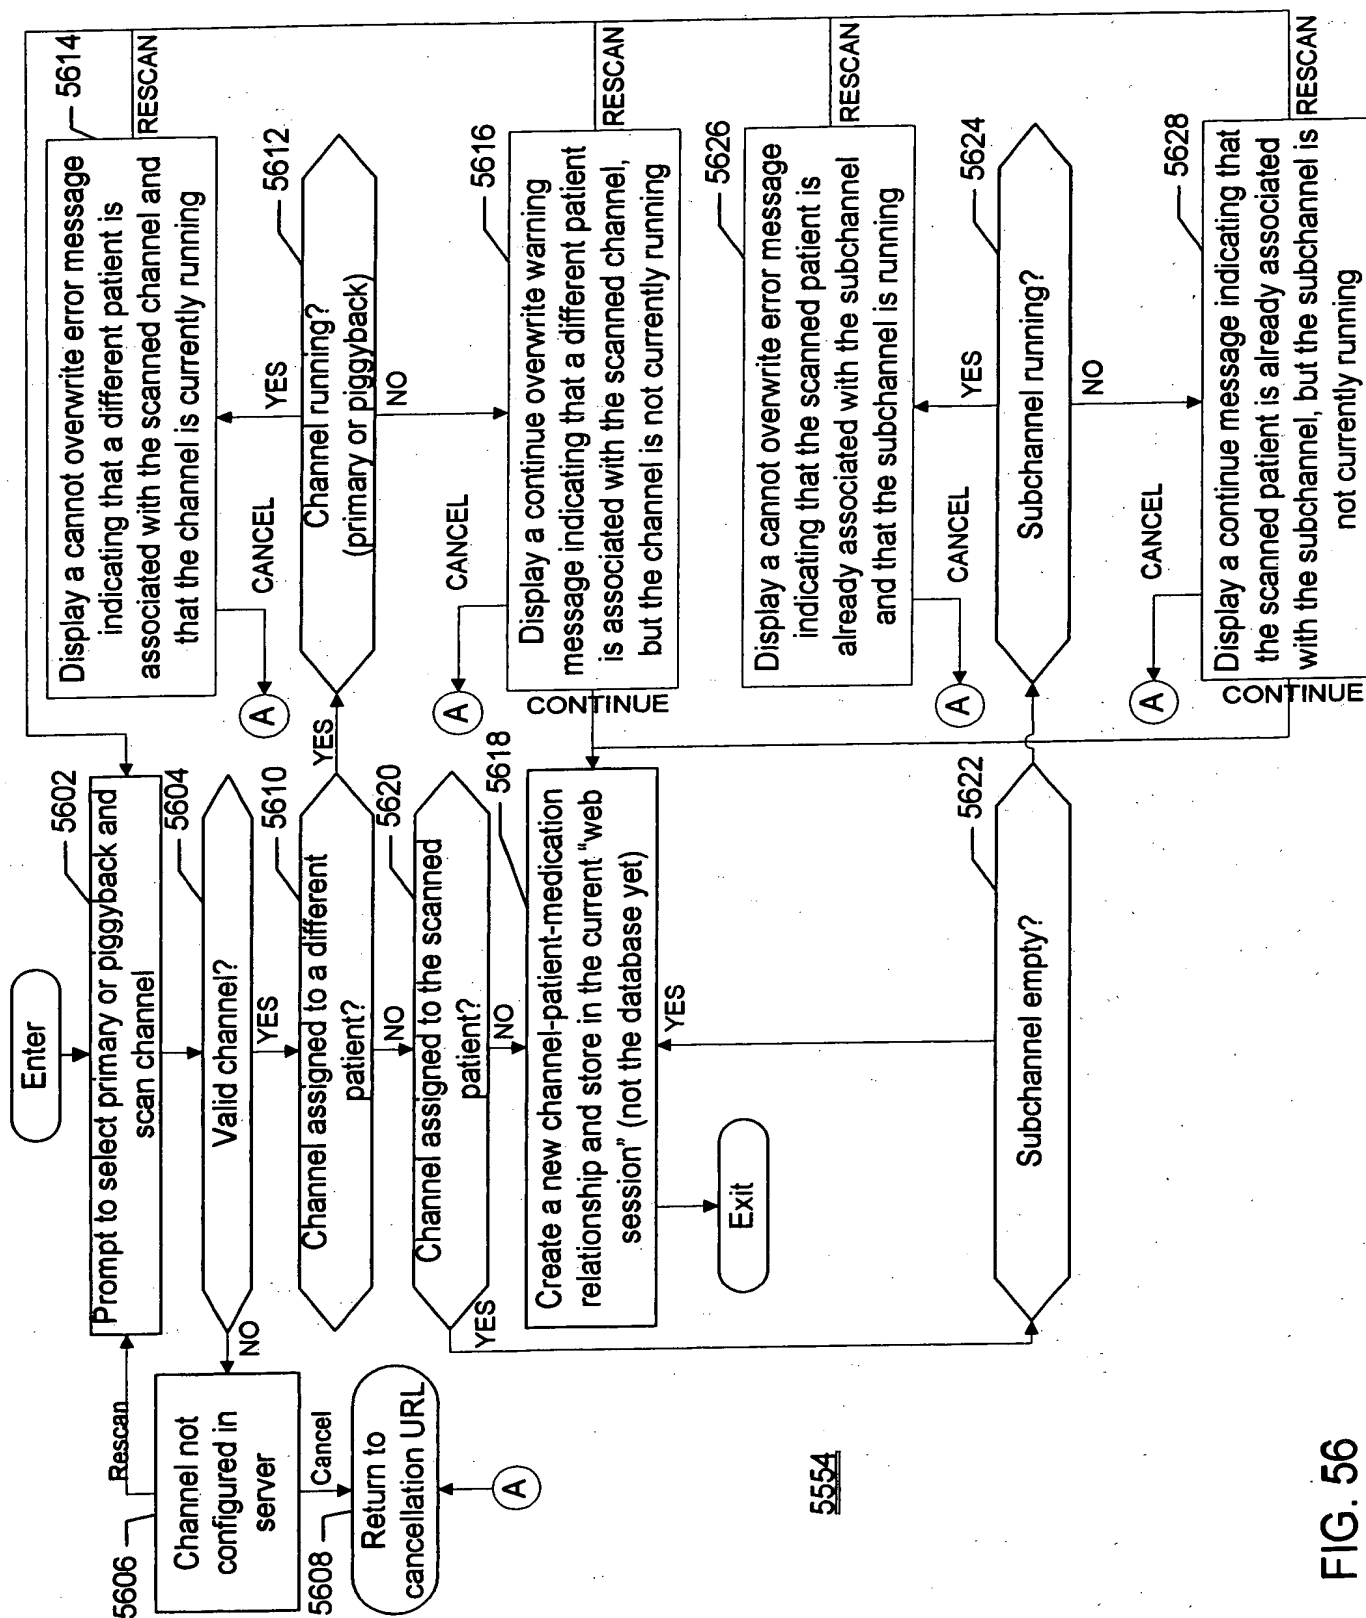


FIG. 56

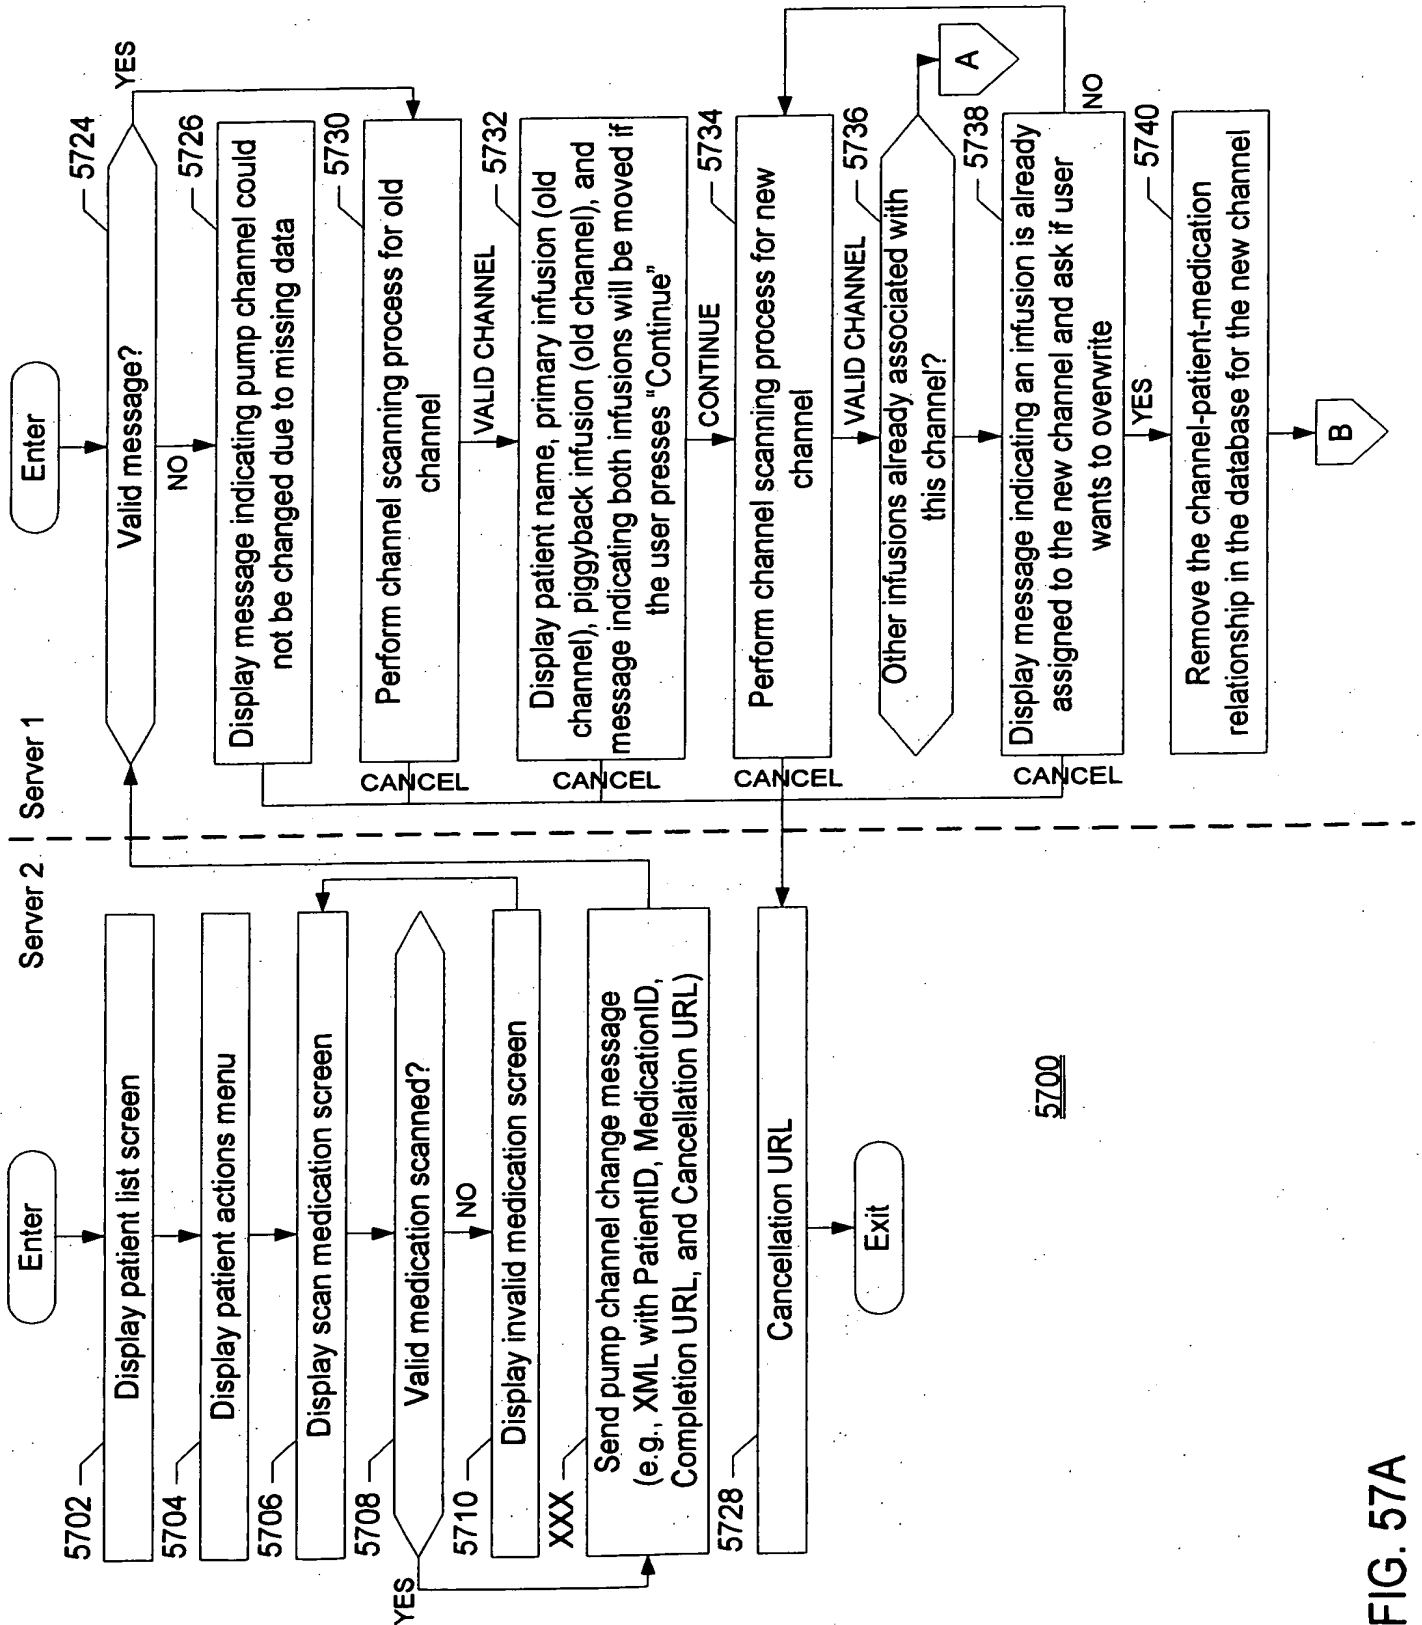


FIG. 57A

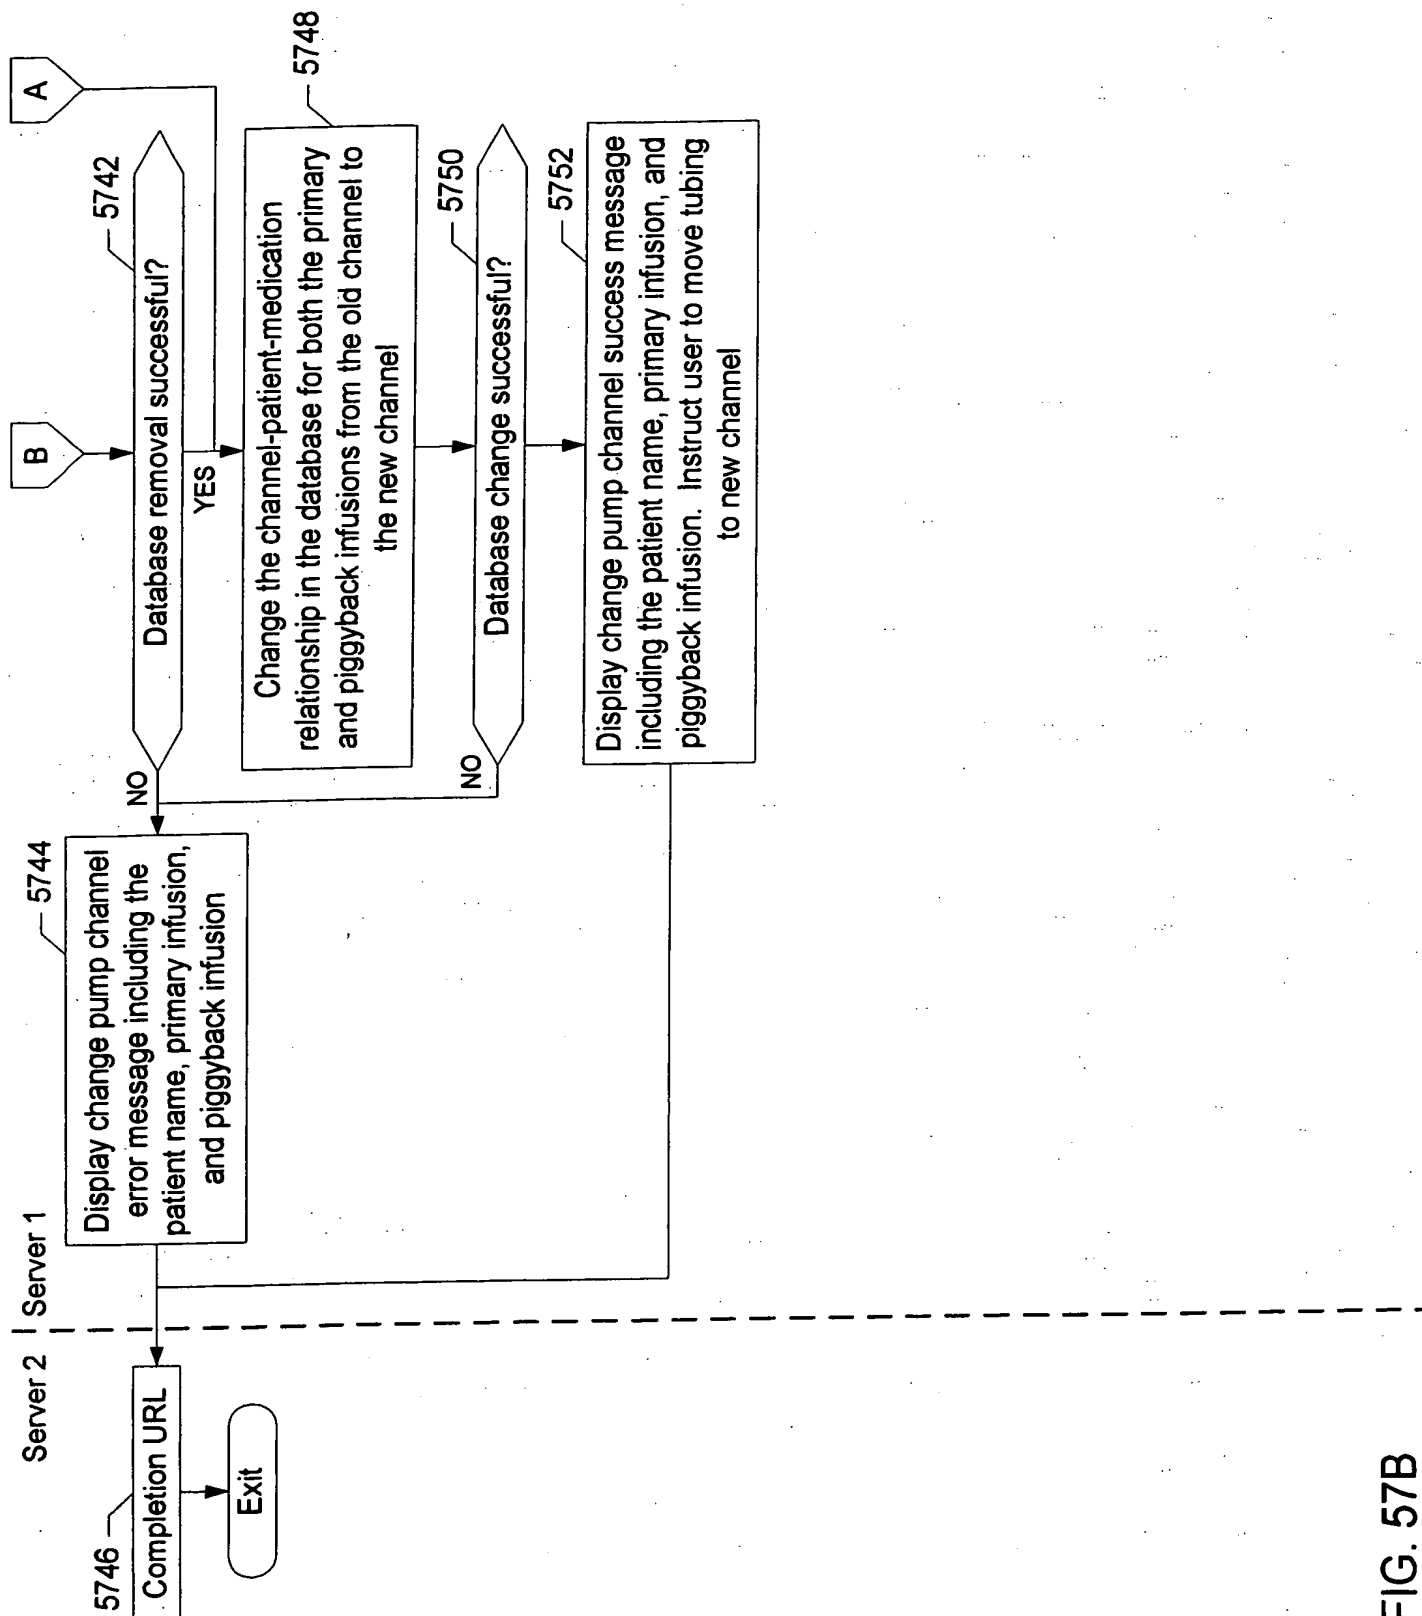


FIG. 57B

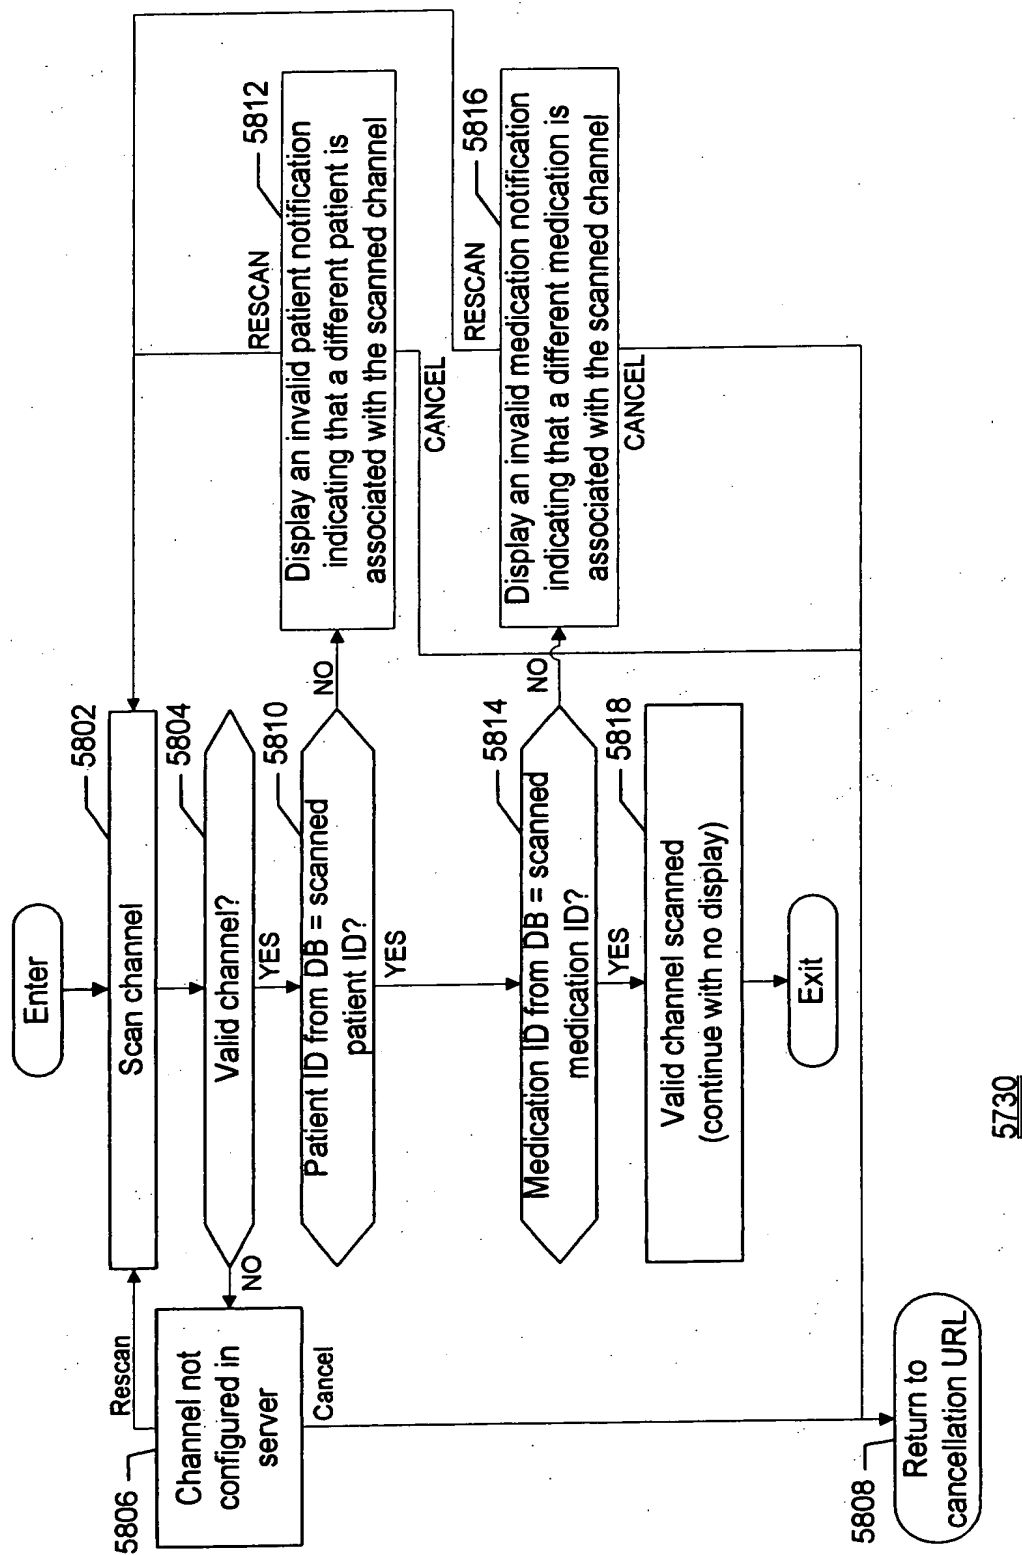


FIG. 58

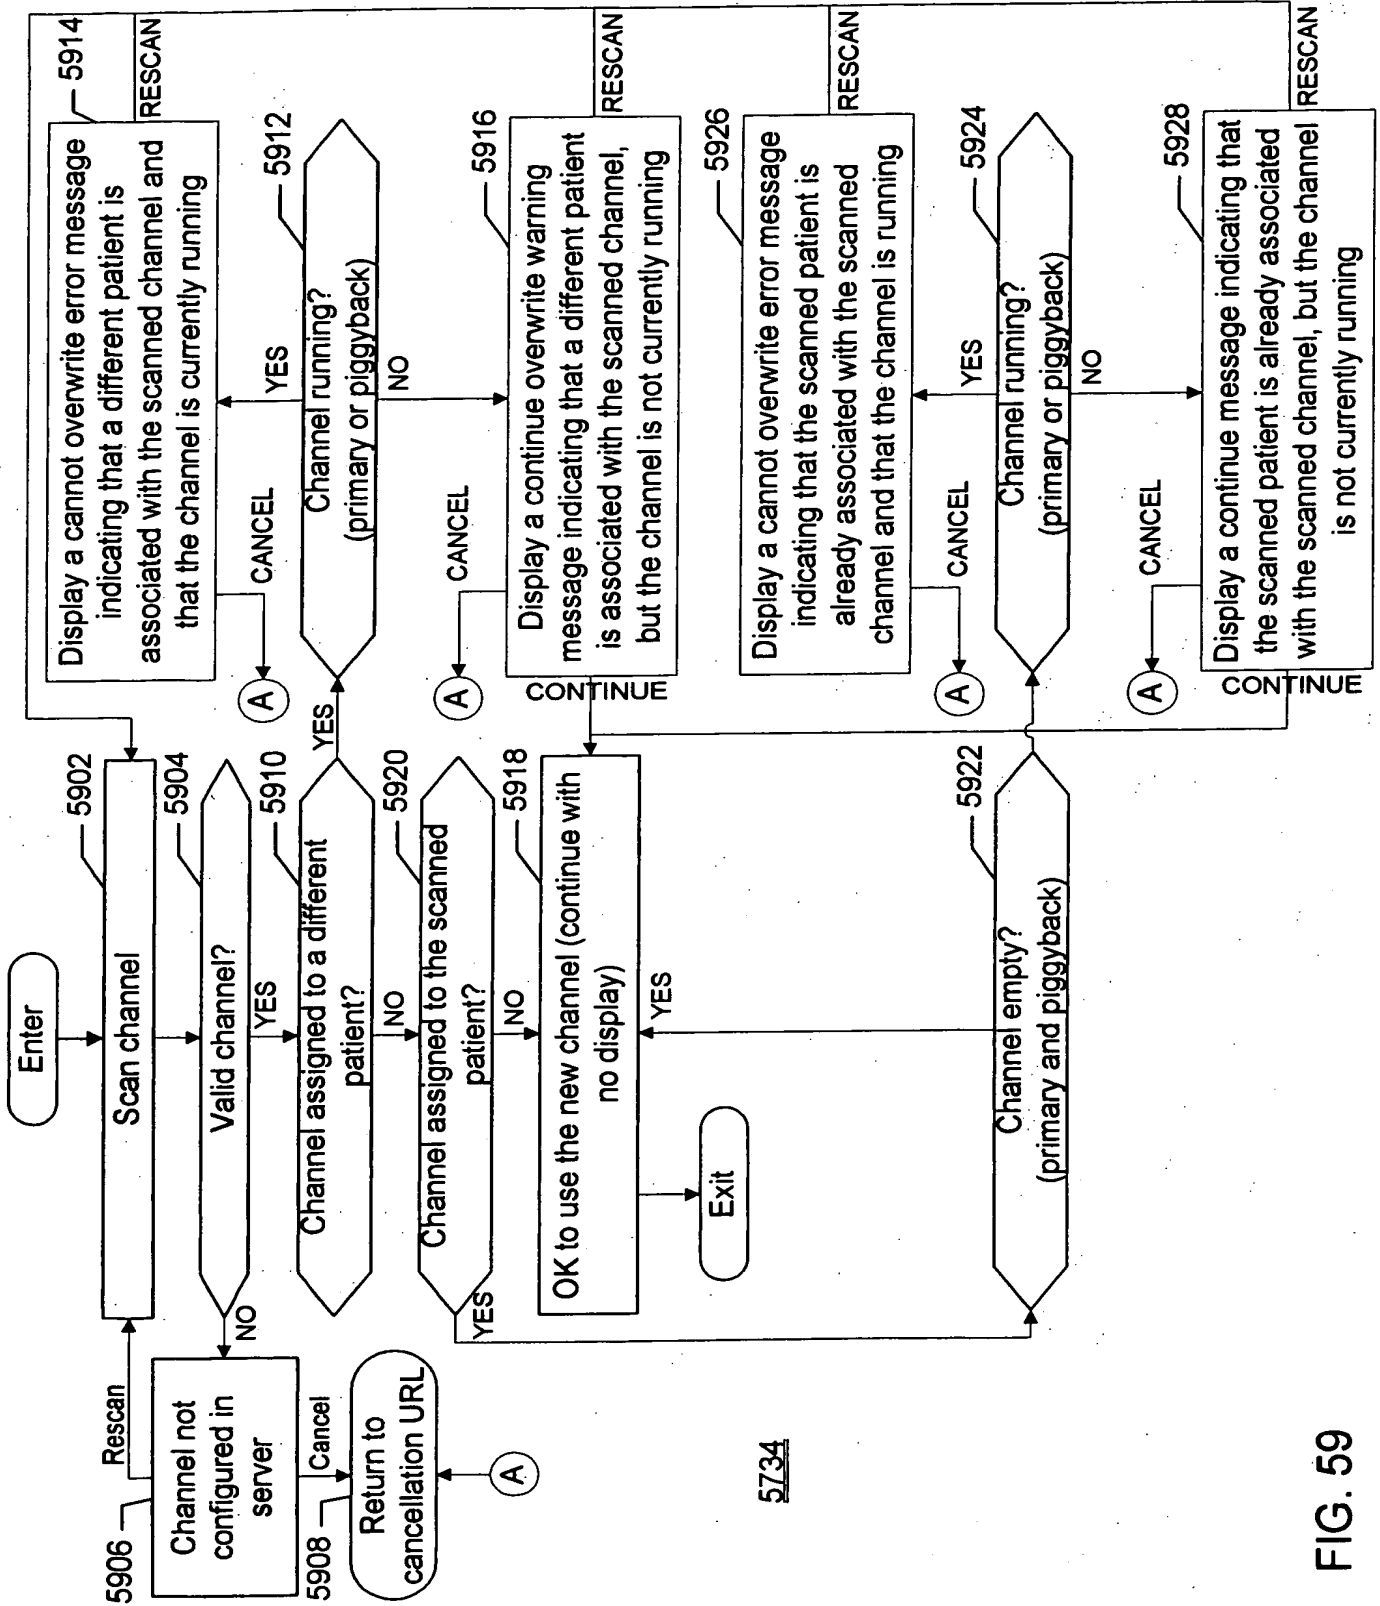


FIG. 59

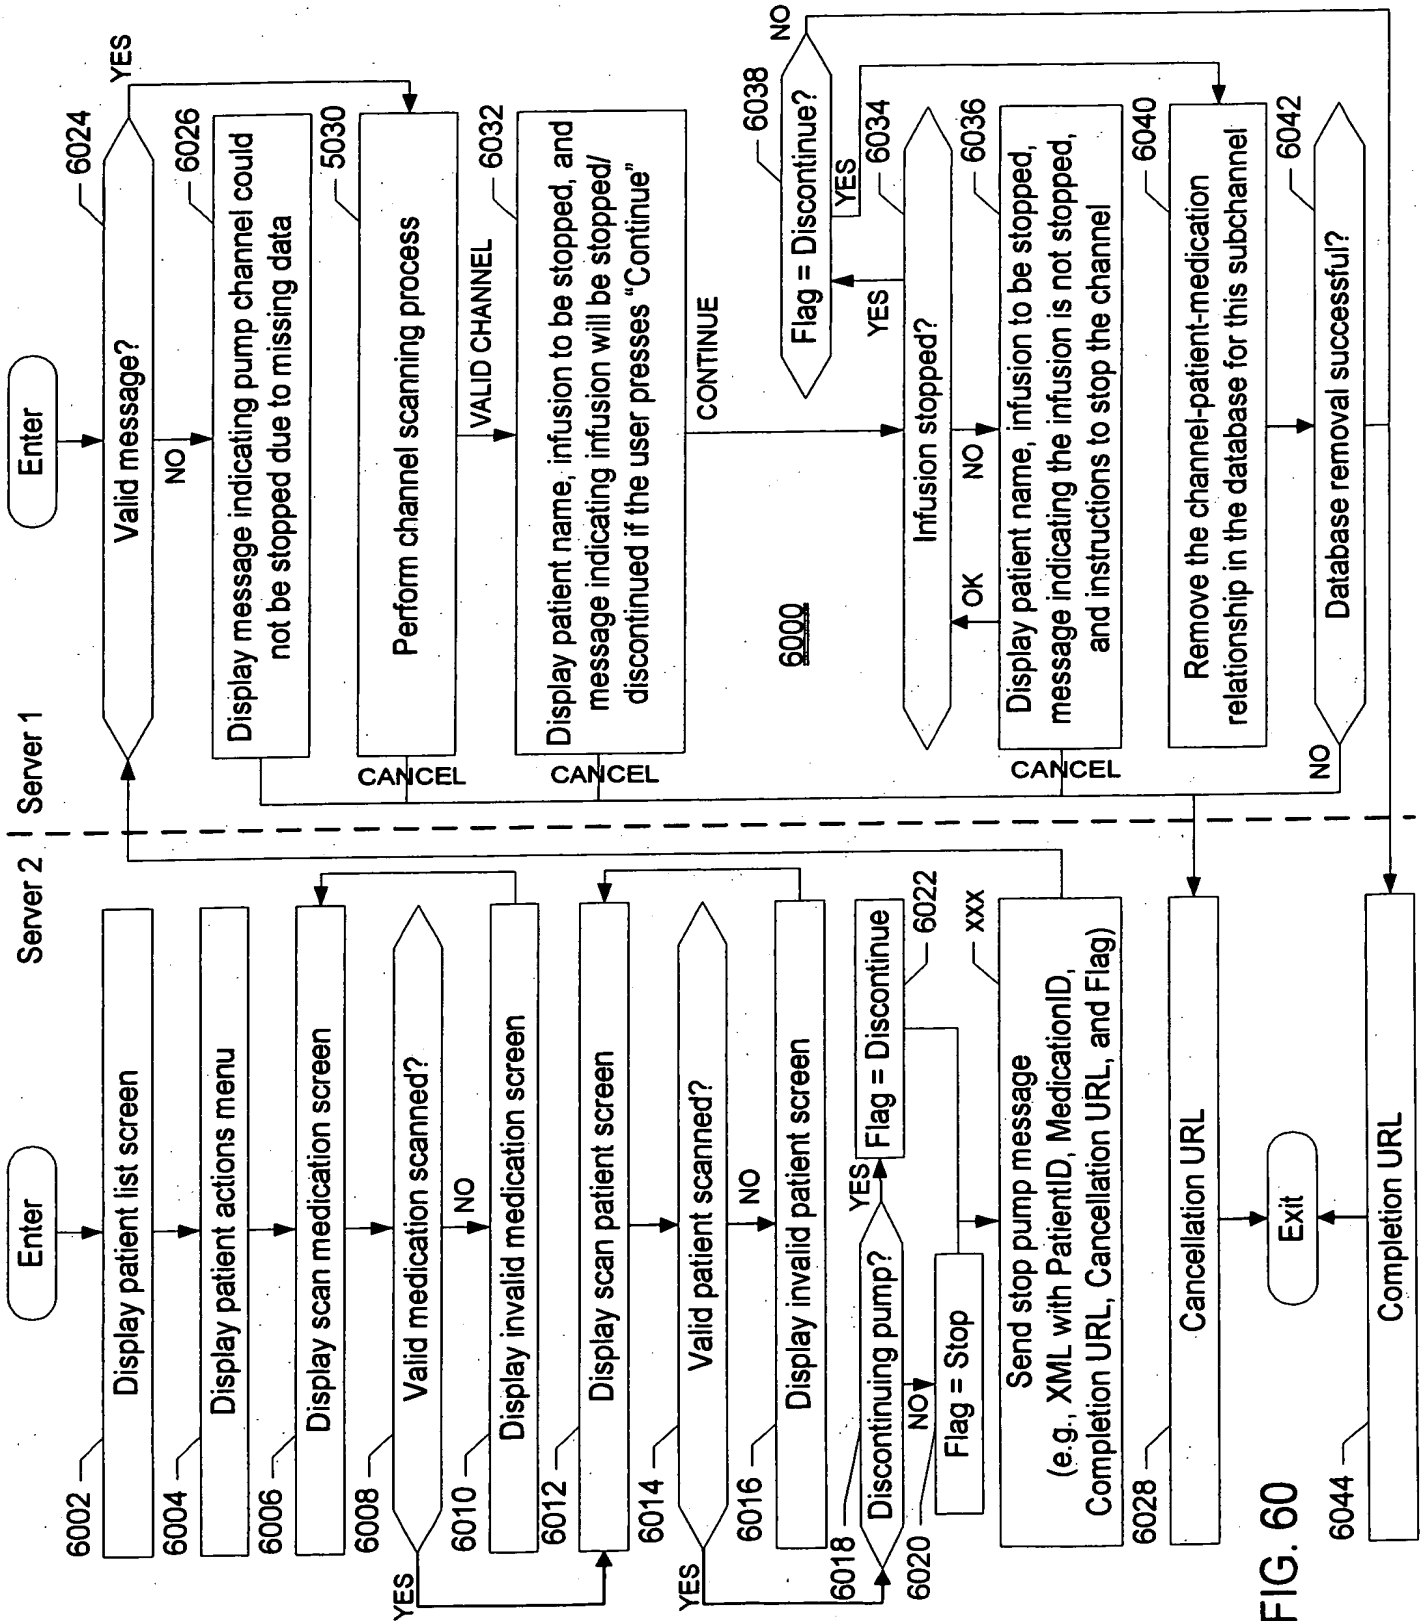


FIG. 60

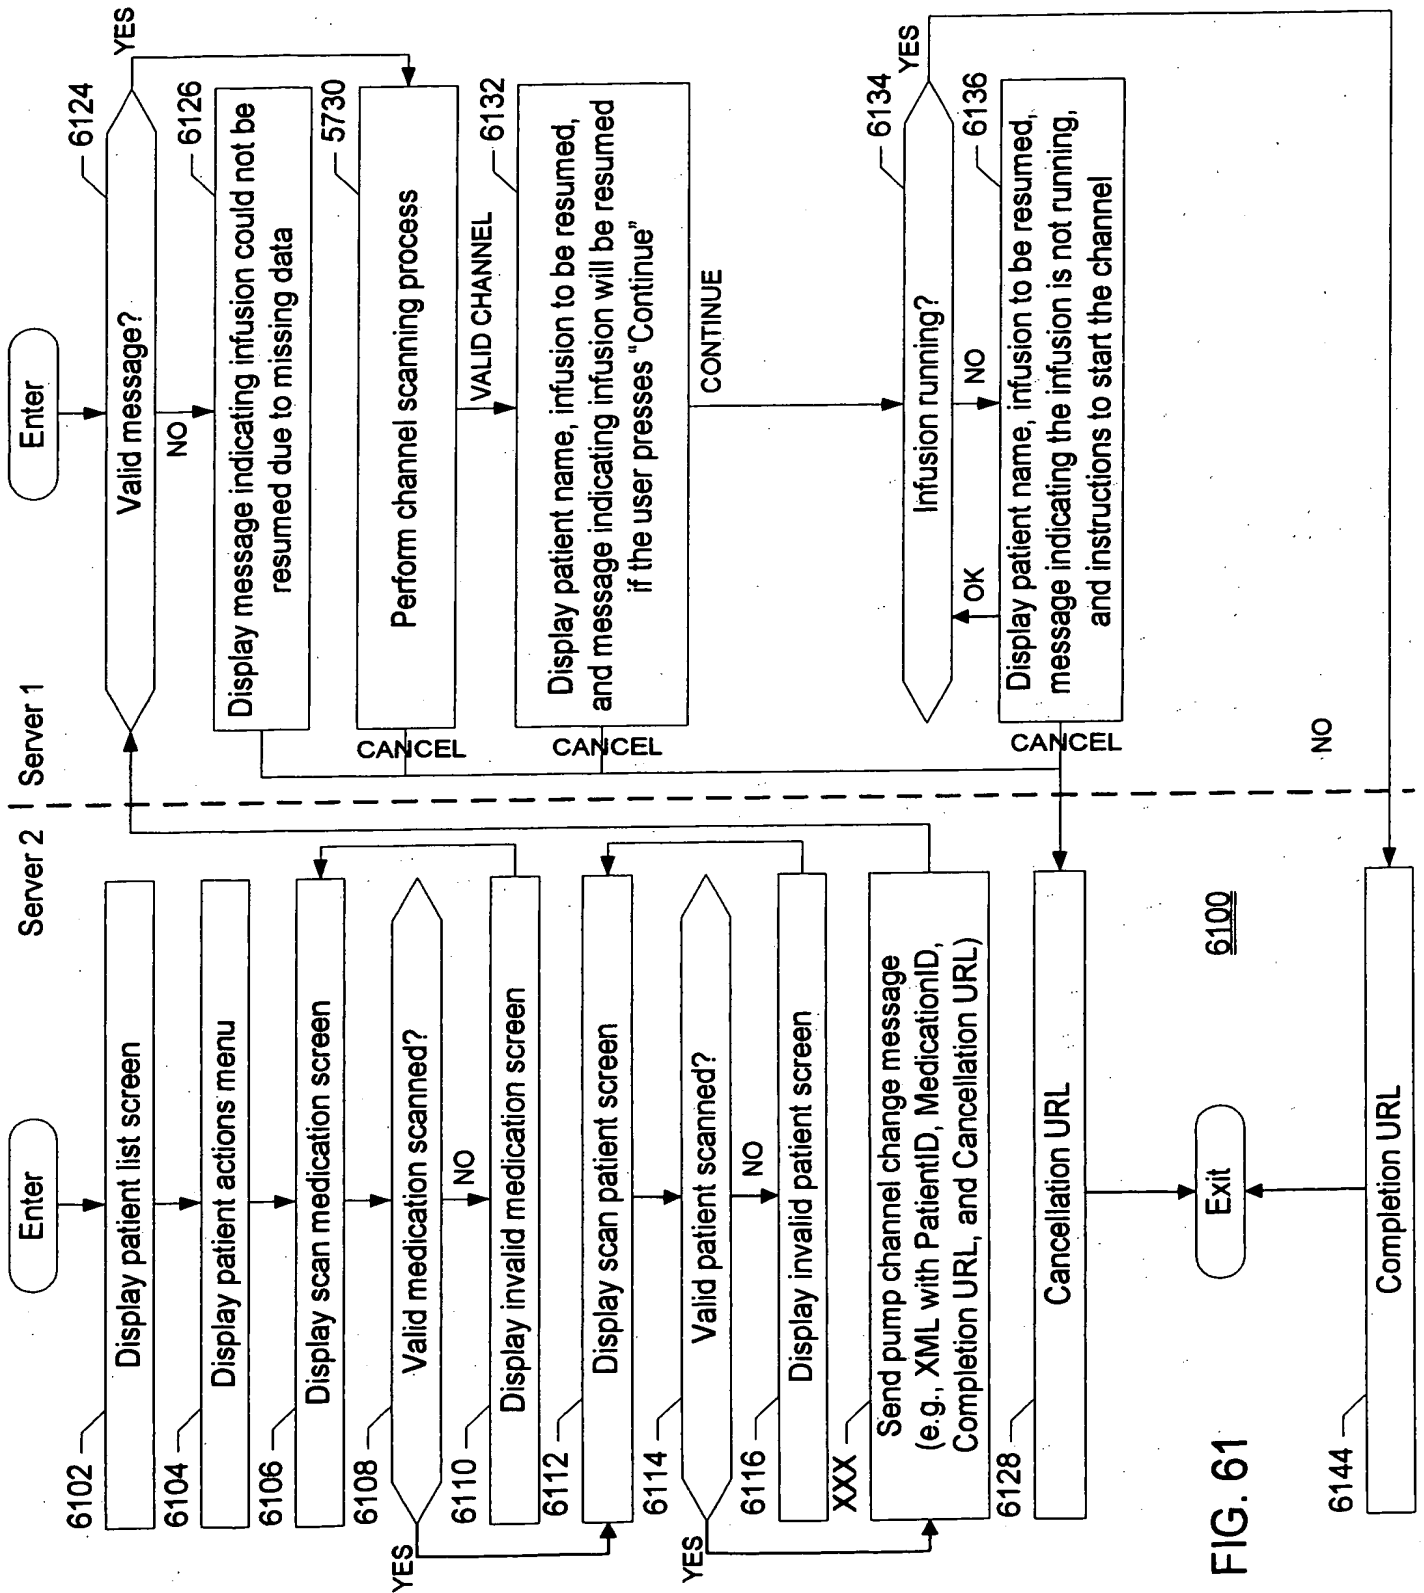


FIG. 61

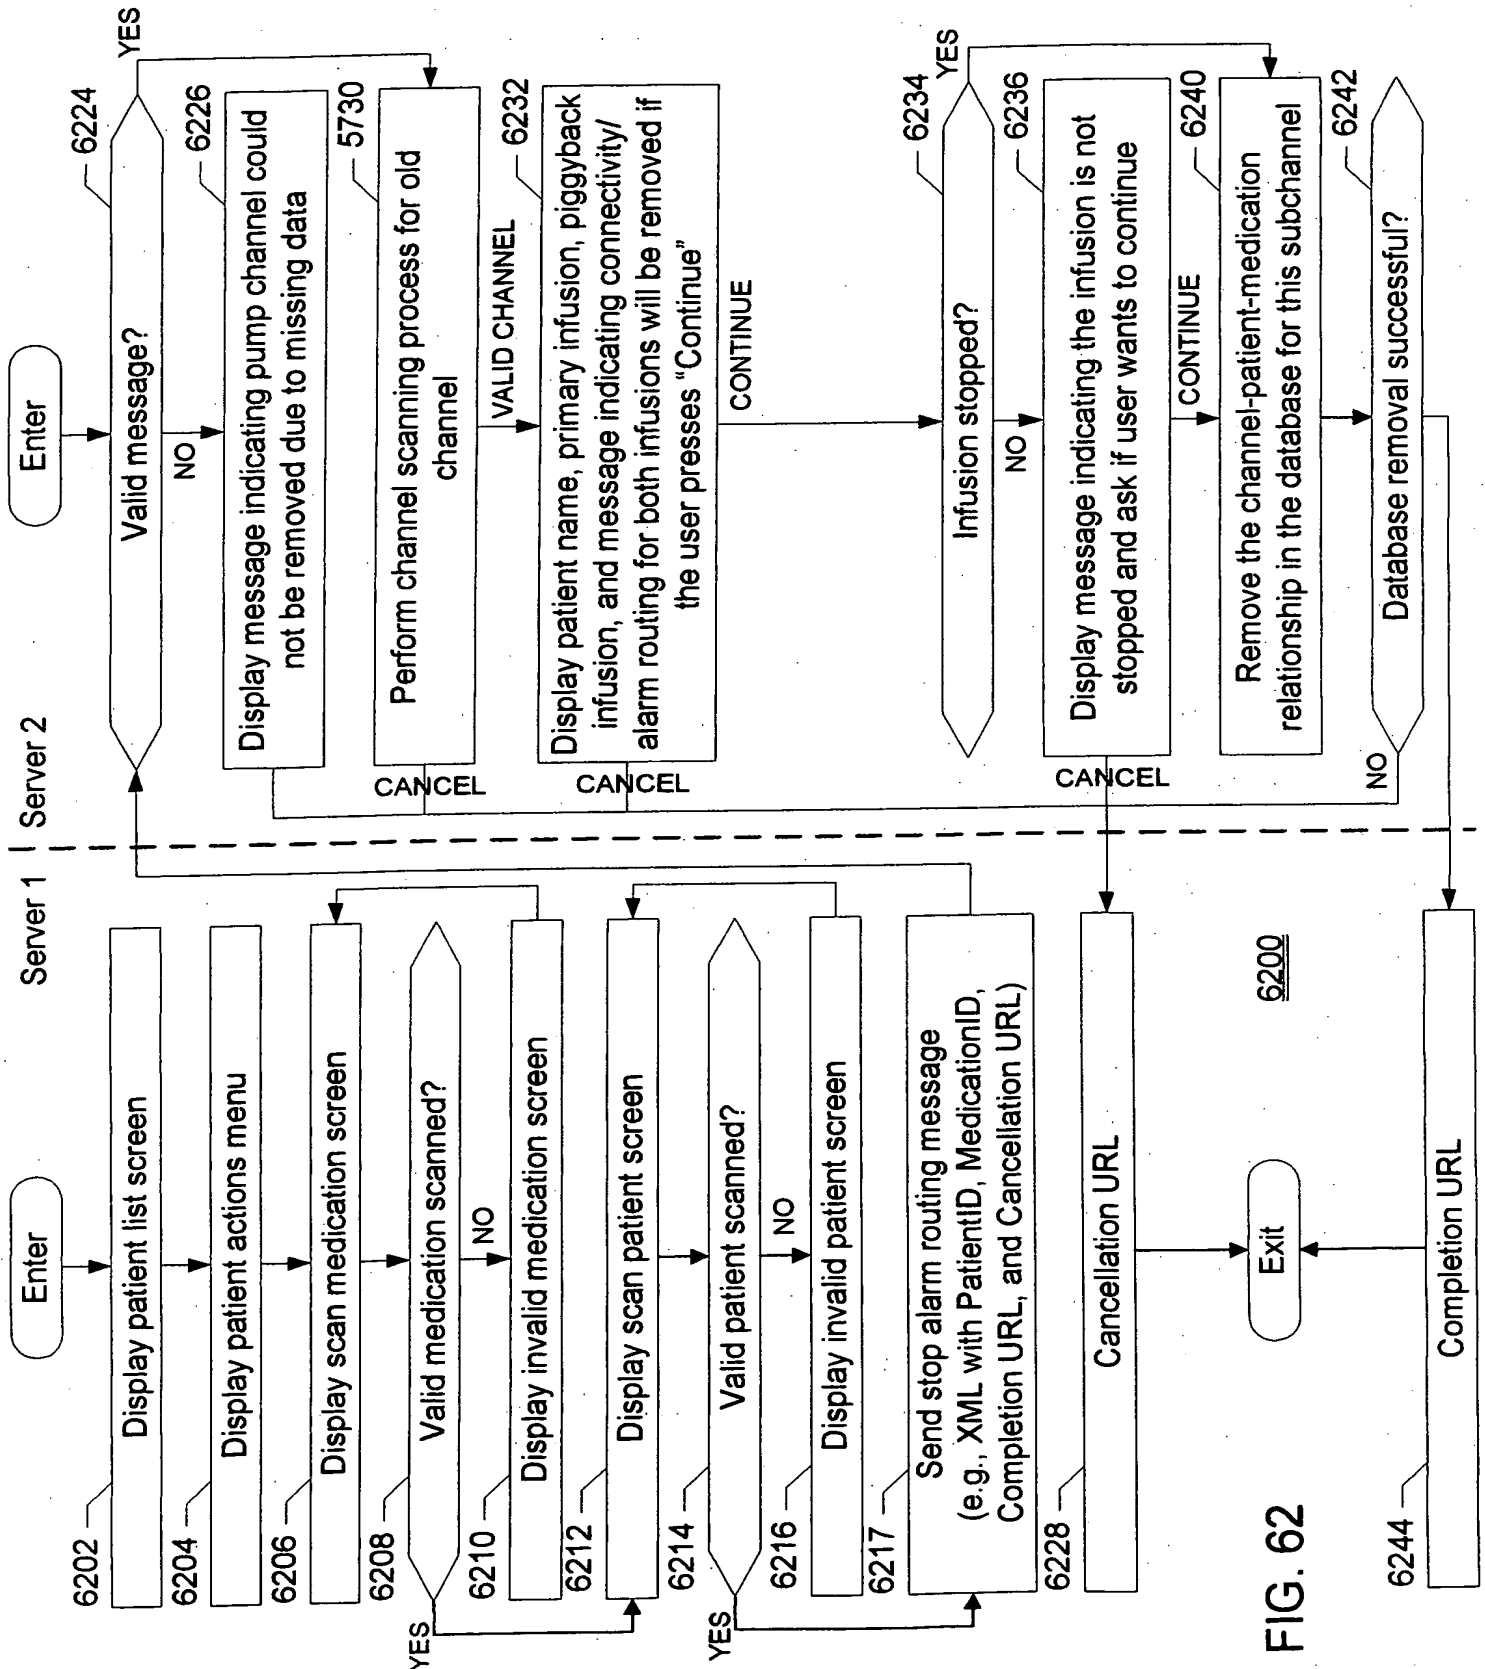


FIG. 62

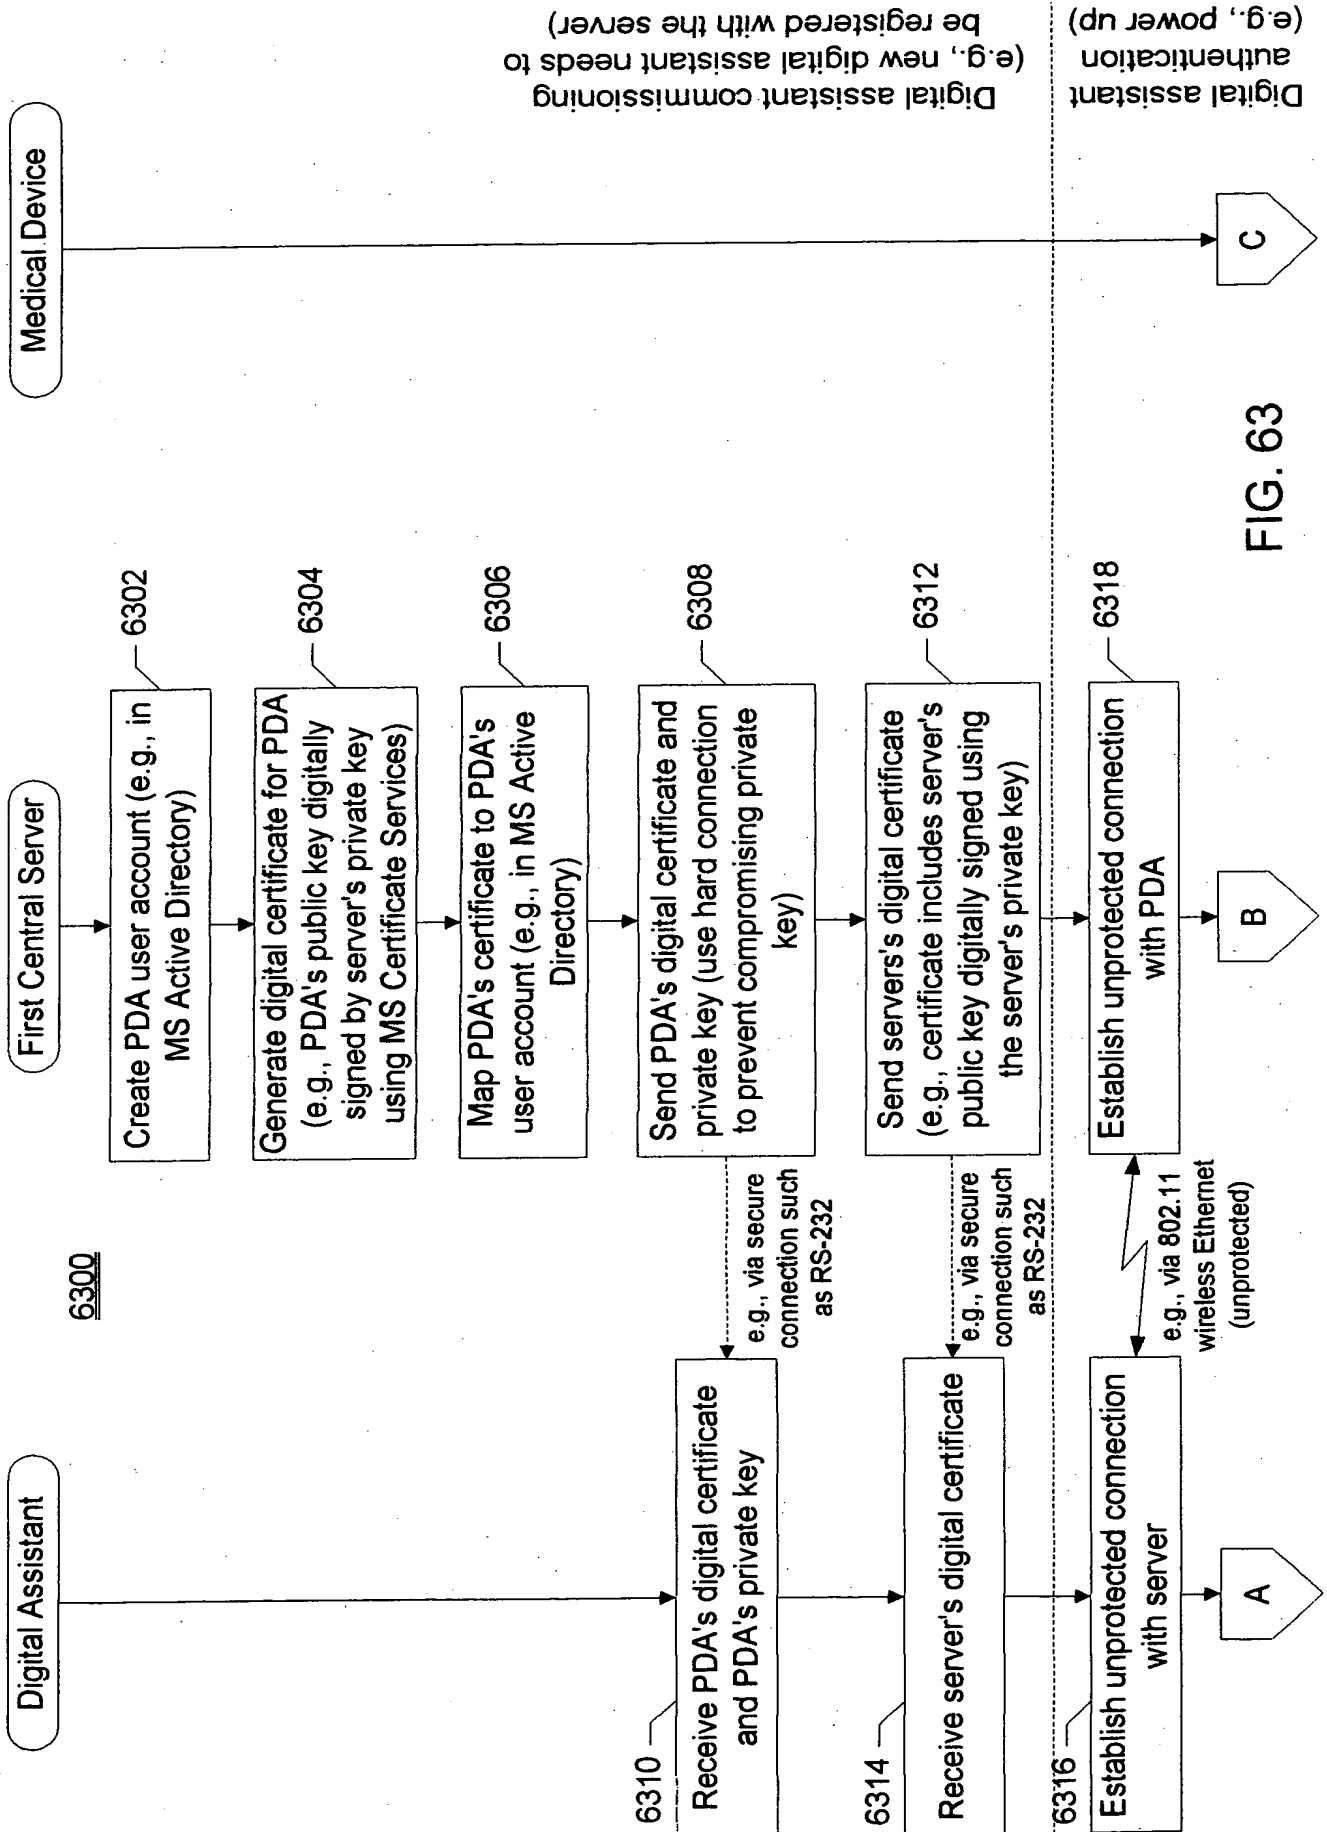


FIG. 63

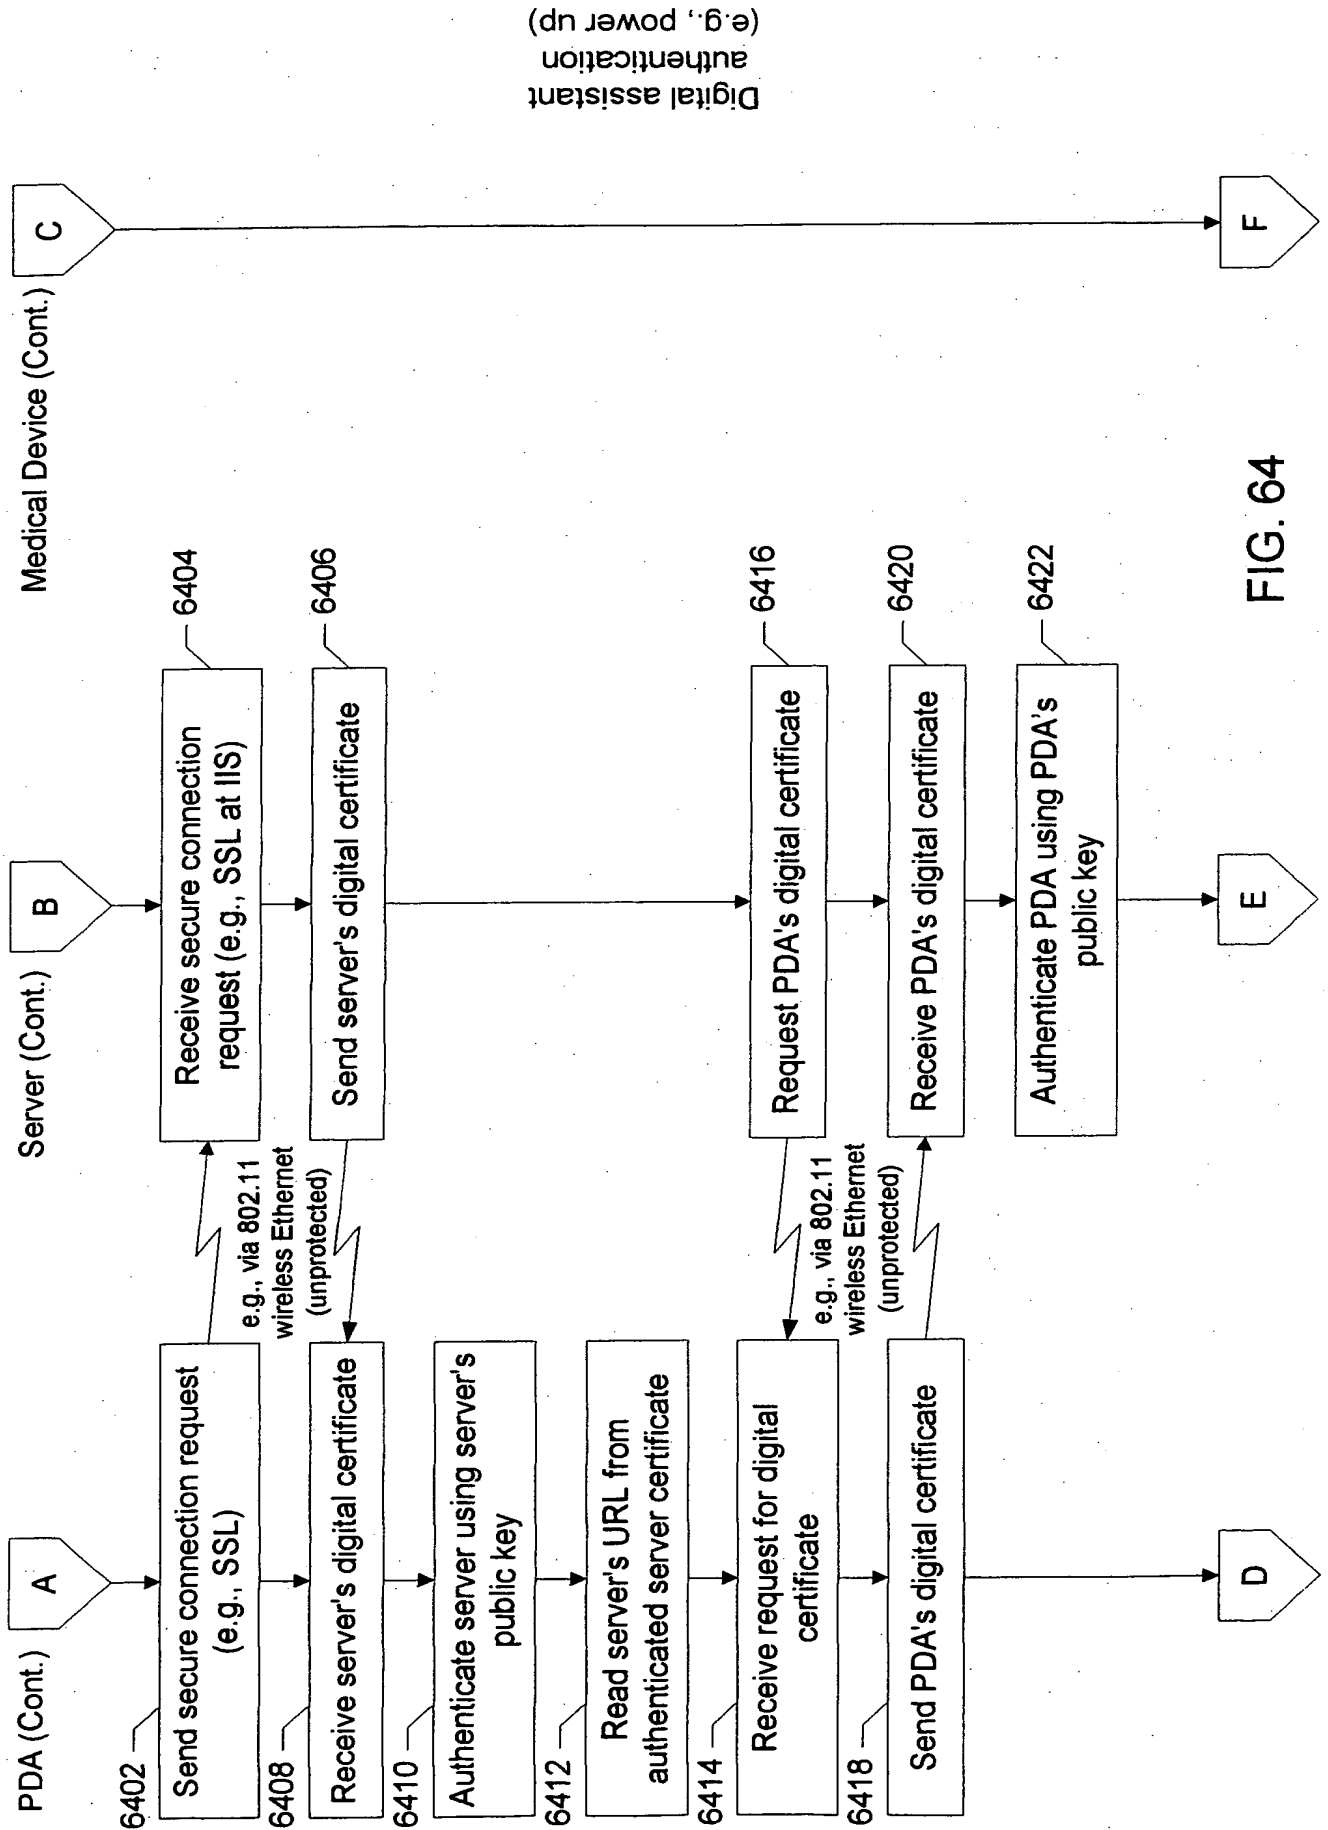


FIG. 64

Digital assistant
authentication
(e.g., power up)

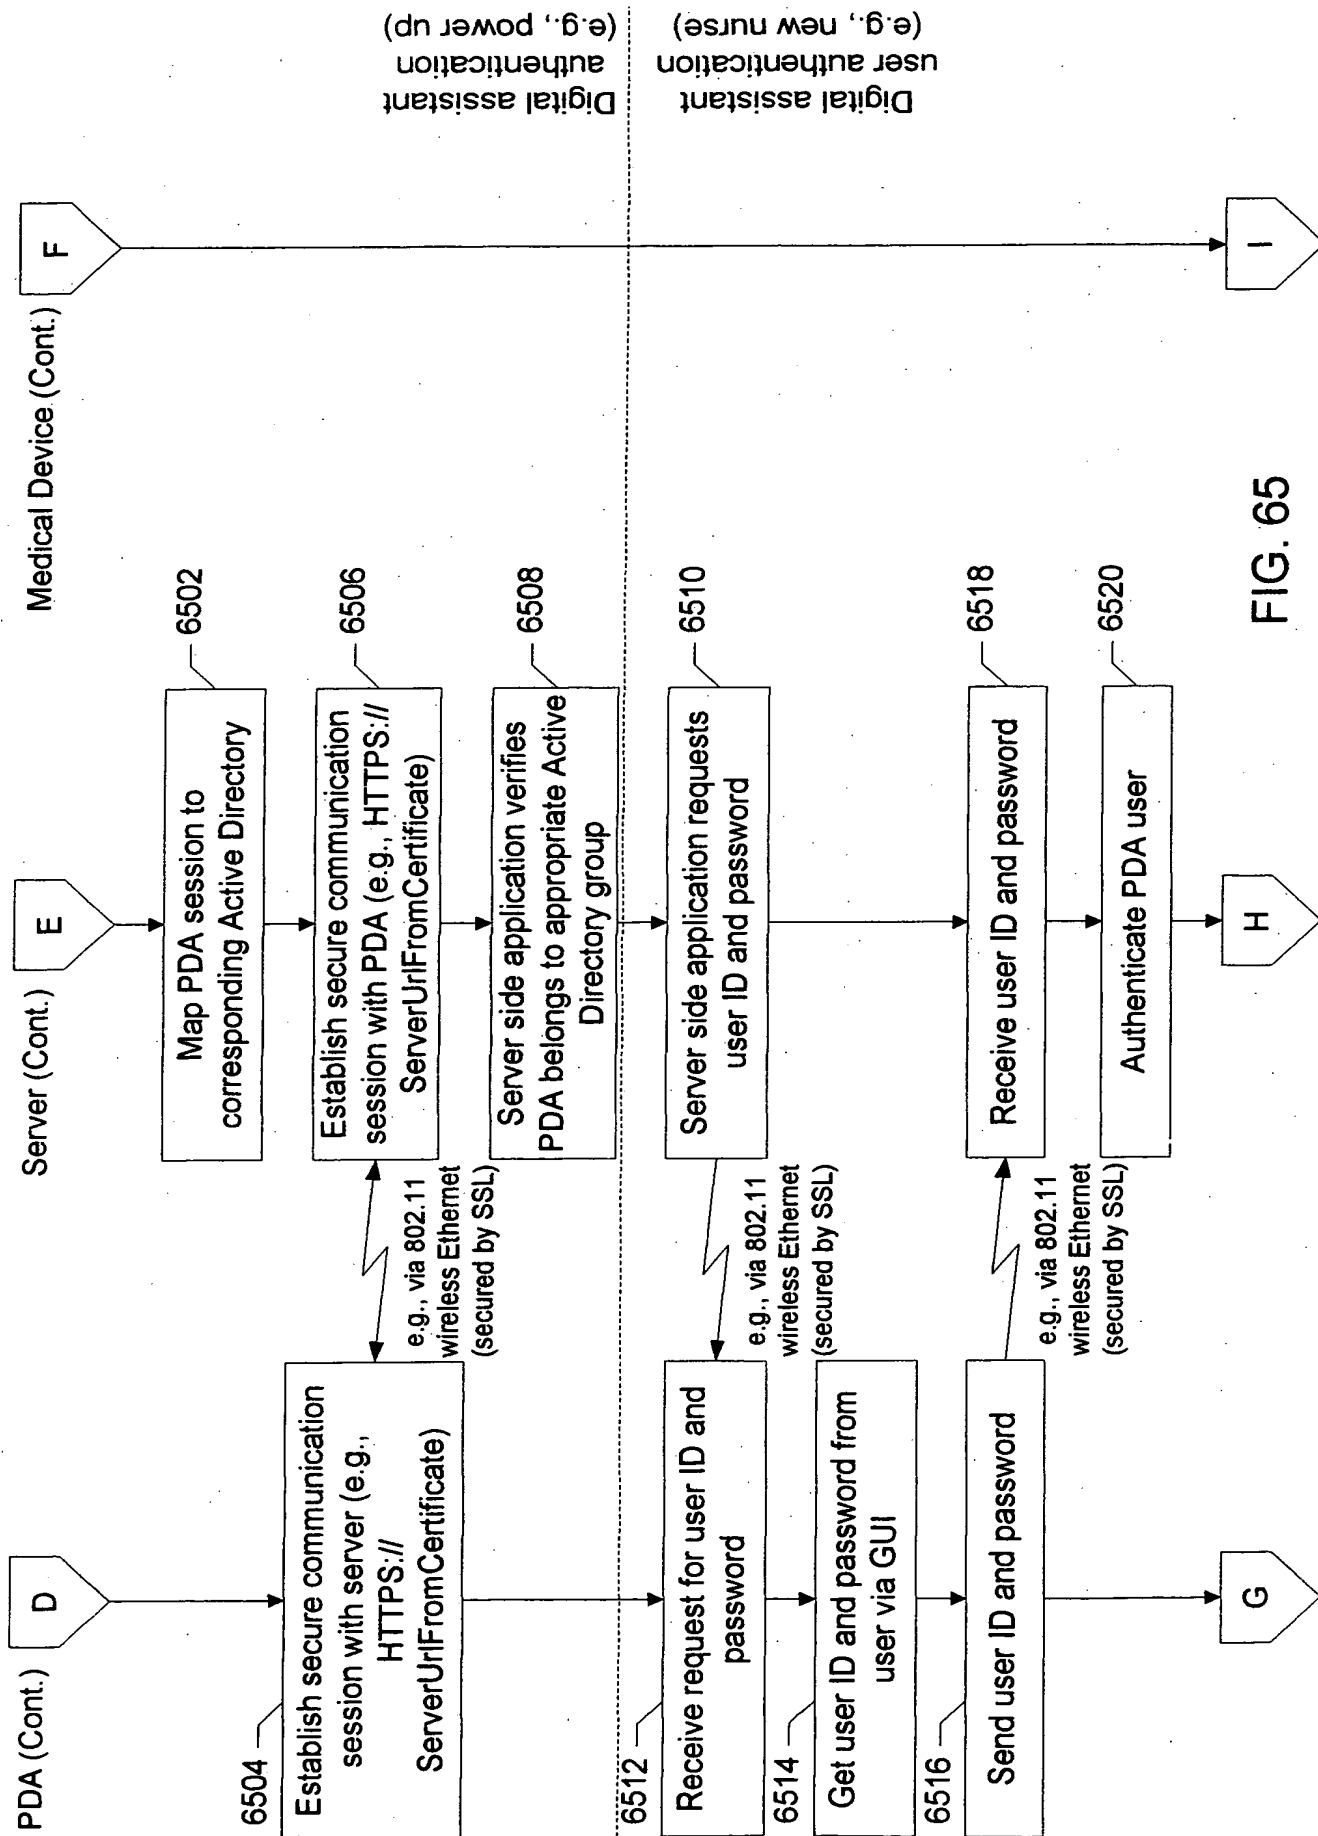


FIG. 65

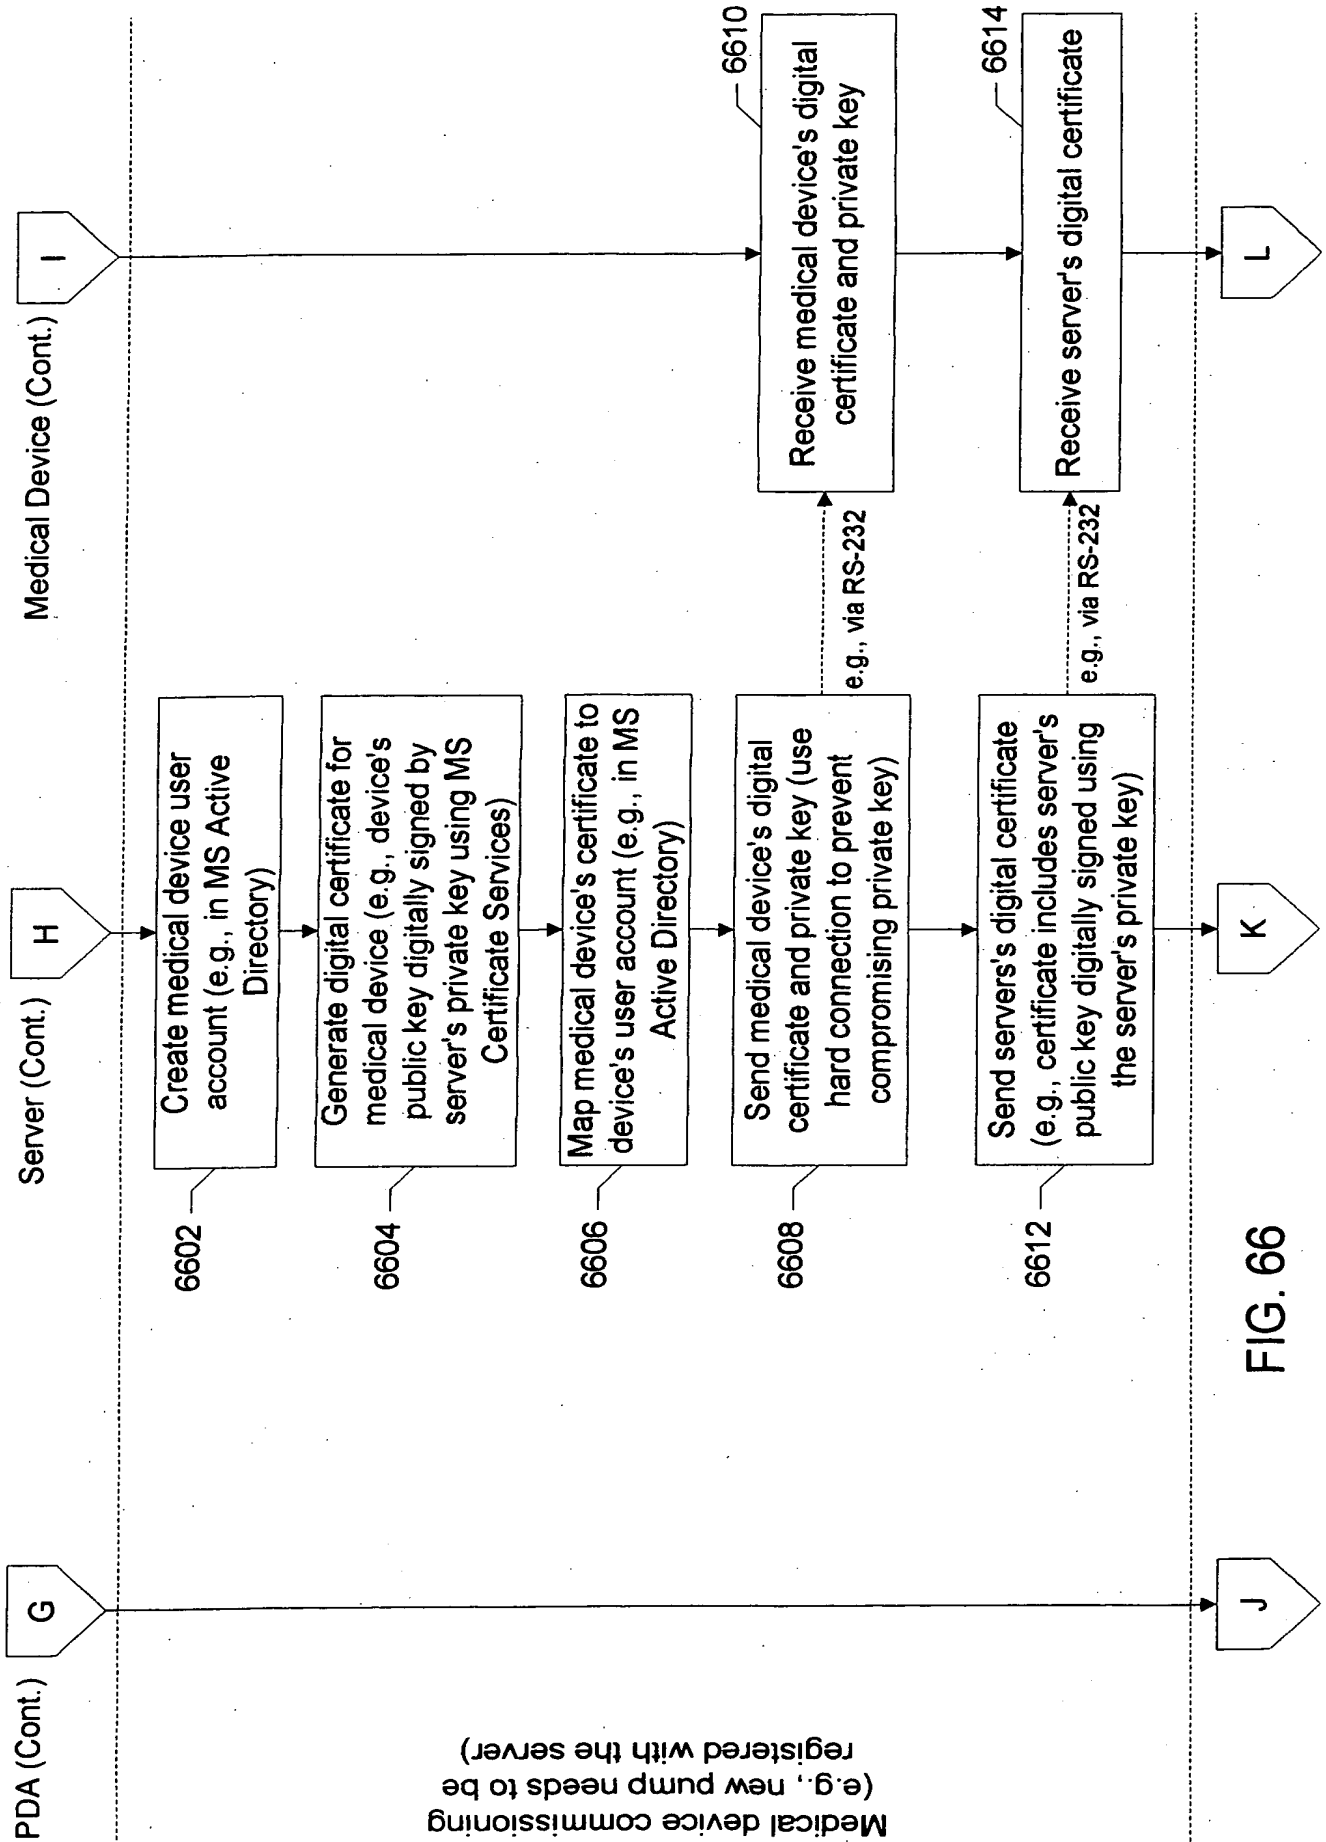


FIG. 66

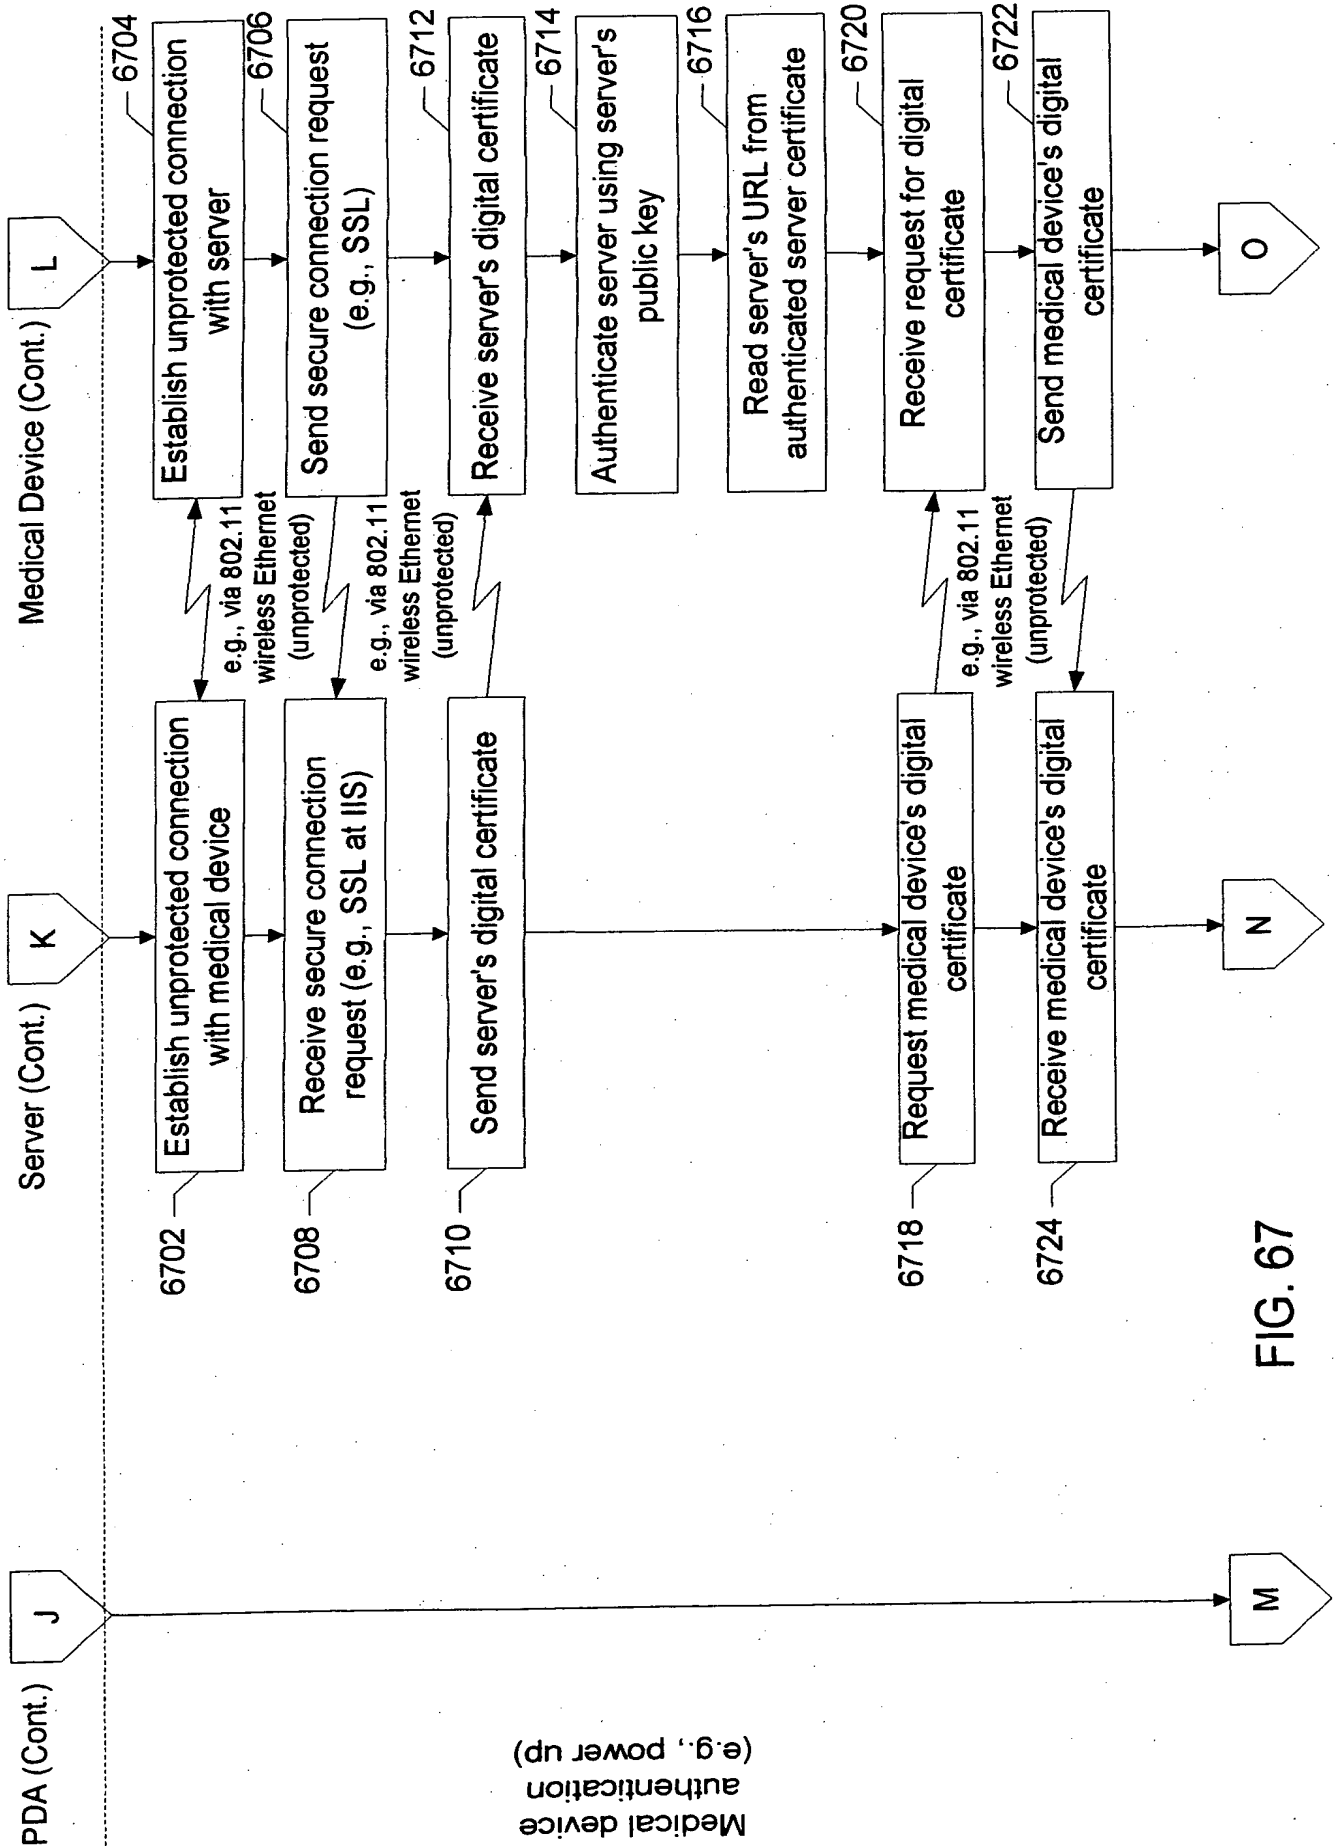


FIG. 67

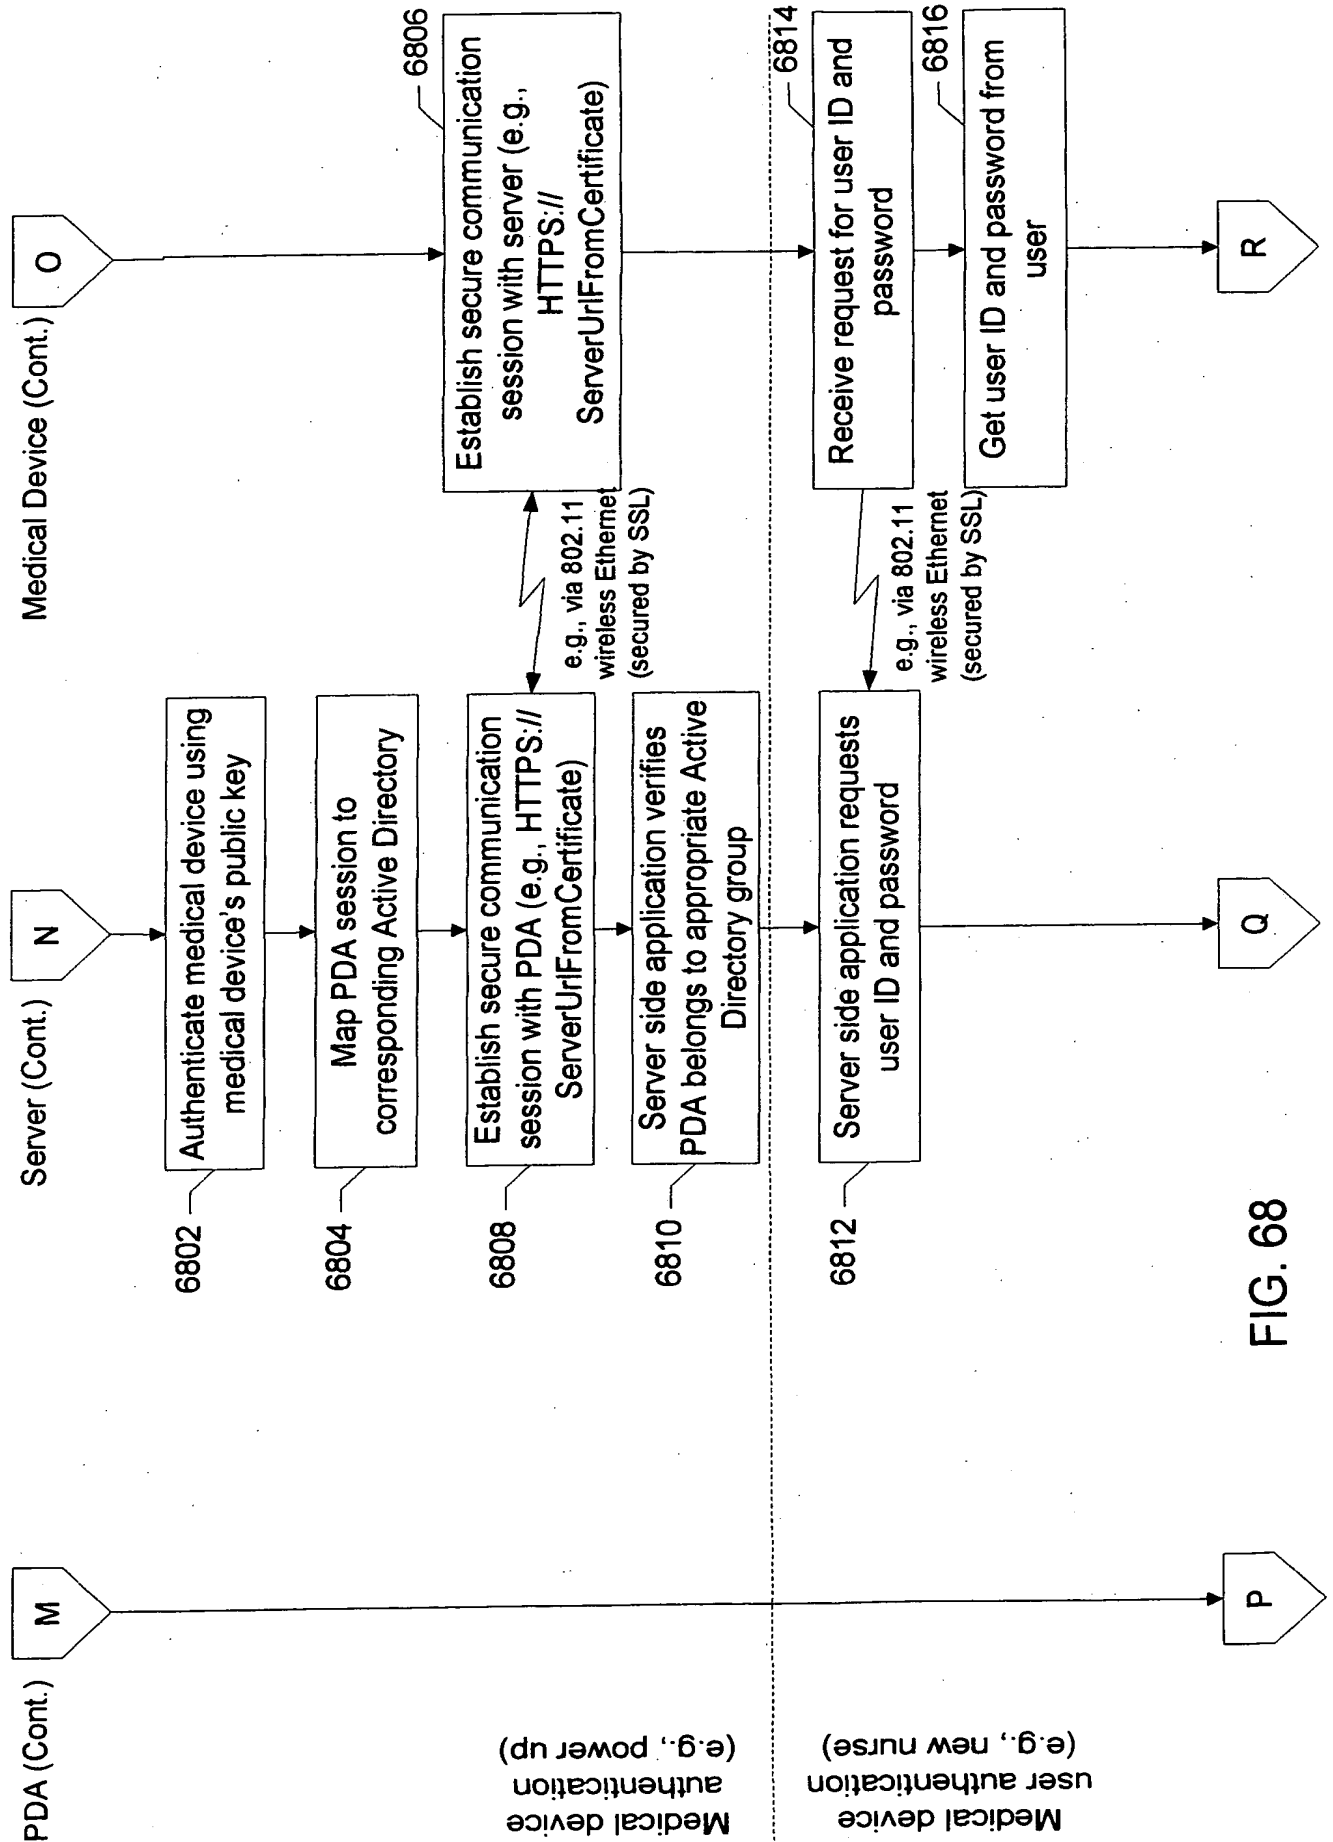


FIG. 68

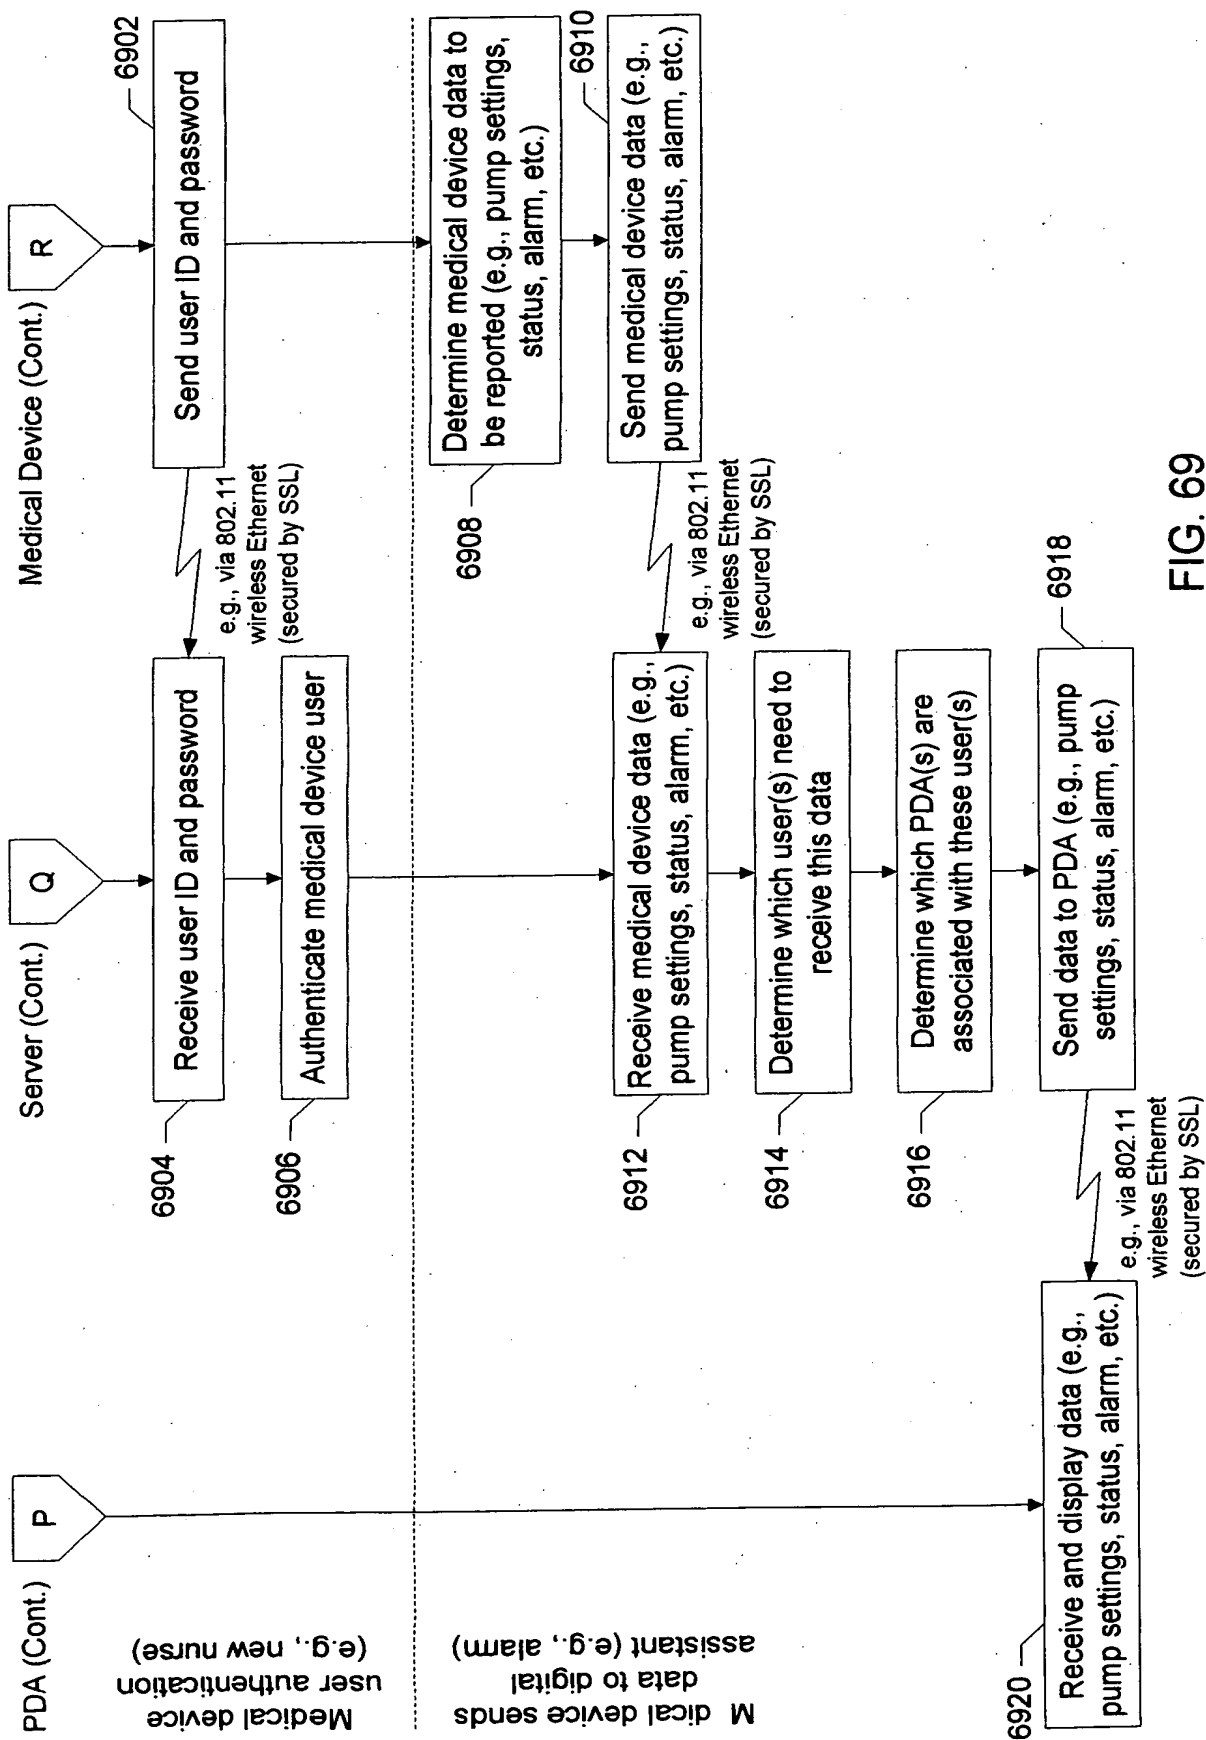


FIG. 69